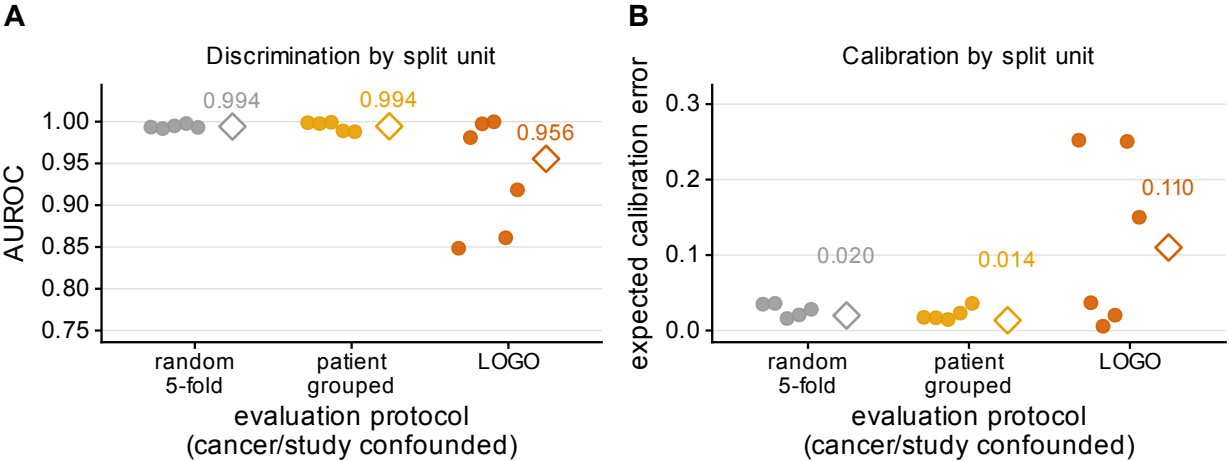
A
Discrimination by split unit
AUROC
1.00
0.95
0.90
0.85
0.80
0.75
0.994
0.994
0.956
random 5-fold
patient grouped
LOGO
evaluation protocol (cancer/study confounded)
B
Calibration by split unit
expected calibration error
0.3
0.2
0.1
0.0
0.020
0.014
0.110
random 5-fold
patient grouped
LOGO
evaluation protocol (cancer/study confounded)