

Can SmO₂ BPs be used as substitute for whole-body thresholds?


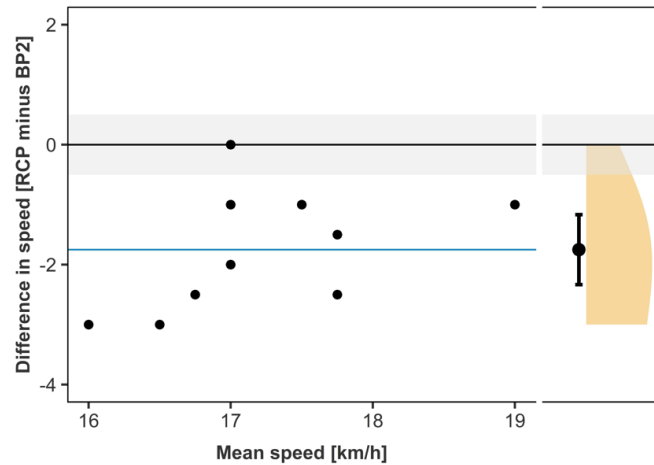


Fig. 3B, Fernández -Jarillo et al. (2026)





→ Real *inter*-individual difference in BPs vs. whole body thresholds

OR

→ Low test-retest reliability of SmO₂ BPs

Methods choice matters

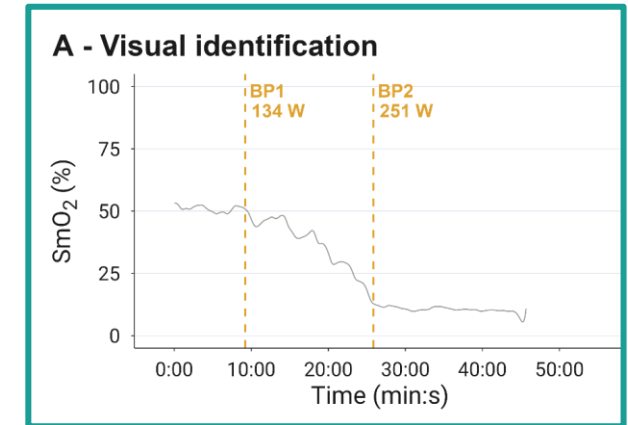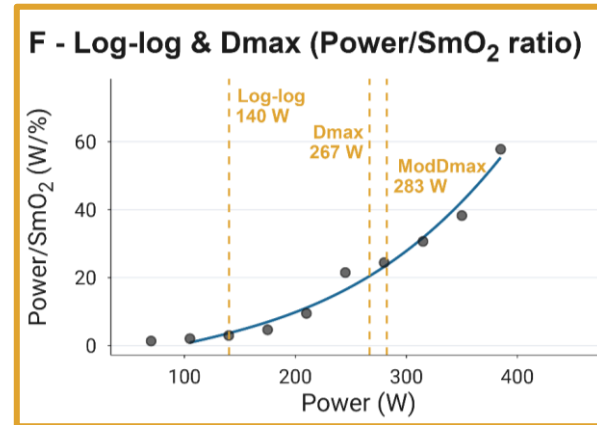

- Not all methods are reliable
- “Best”: **Log-log & Dmax on Power/SmO₂ ratio**
- **Visual identification** among most reliable methods
- Consider **reliability** and *physiological validity*
- Side differences are small – **one NIRS device may be sufficient**