


Sample: T2IS1
 Operator: LvdM, ChemEng, Stb Uni
 Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
 File: C:\...\RHASCH~1\005-953.SMP

Test Number: 3
 Analyzed: 2026/06/18 11:45:44PM
 Reported: 2026/06/29 9:30:43PM
 Background: 2026/06/18 10:38:57PM

Model: (1.520, 0.1000000), 1.331
 Material: Sand / Water
 Background: Water RI 1.331
 Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.7%

Combined Report

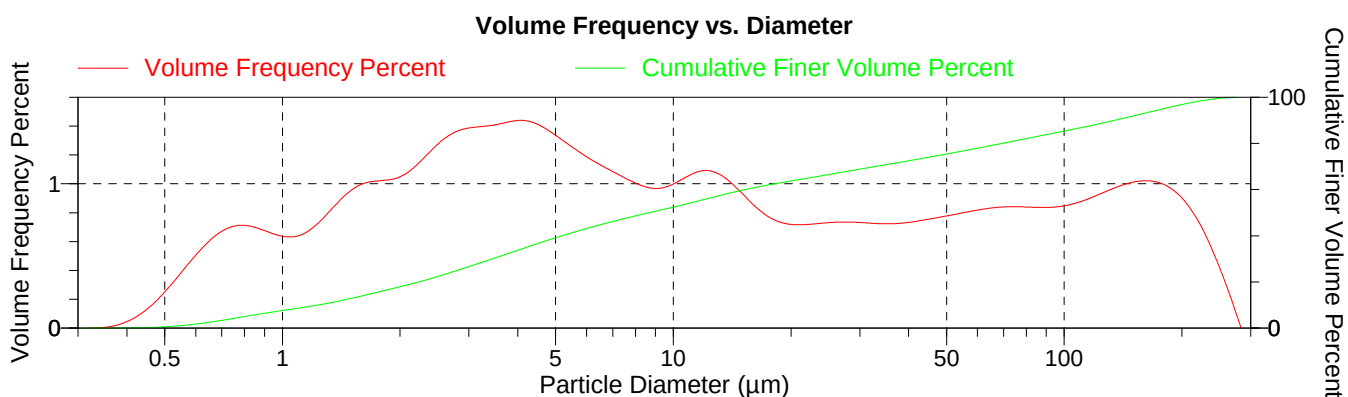

Summary Report

Analysis Conditions

FlowRate: 12.0 l/m
 Circulation time: 60 sec

Ultrasonic intensity: 60 %
 Ultrasonic time: 75 sec

Sample

Sample Concentration: 0.00311 %
 Obscuration: 11.4 %

Volume Distribution Arithmetic Statistics

		Std Dev of 3			Std Dev of 3
Mean	38.31	1.582	Mode	4.005	0.000
Median	8.677	0.088			

Selected Sizes

Diameter (µm)	Percent Finer
100.0	85.4
50.00	75.4
20.00	63.7
10.00	52.4
1.000	7.6

Peaks

Peak Number	% of Dist.*	% of Dist. Std Dev of 3	Mean	Mean Std Dev of 3	Median	Median Std Dev of 3	Mode
1	8.6	N/A	0.764	N/A	0.758	N/A	0.799
2	42.4	N/A	3.903	N/A	3.419	N/A	4.005
3	13.8	N/A	14.17	N/A	13.50	N/A	11.96
4	6.6	N/A	28.66	N/A	28.35	N/A	26.77
5	12.8	N/A	61.05	N/A	59.43	N/A	75.45
6	15.8	N/A	157.9	N/A	151.7	N/A	159.5

* Peaks must comprise at least 5.00 % of the distribution.

Sample: T2IS1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-953.SMP

Test Number: 3
Analyzed: 2026/06/18 11:45:44PM
Reported: 2026/06/29 9:30:43PM
Background: 2026/06/18 10:38:57PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.7%

Report by Size Table

Low Diameter (μ m)	Cumulative Volume Finer (Percent)	Low Diameter (μ m)	Cumulative Volume Finer (Percent)	Low Diameter (μ m)	Cumulative Volume Finer (Percent)	Low Diameter (μ m)	Cumulative Volume Finer (Percent)
250.000	99.6	50.000	75.4	7.000	46.2	0.800	5.0
200.000	96.9	40.000	72.5	6.000	43.1	0.700	3.3
150.000	91.9	30.000	68.9	5.000	39.2	0.600	1.7
100.000	85.4	25.000	66.5	4.000	33.7	0.500	0.6
90.000	83.8	20.000	63.7	3.000	26.7	0.400	0.0
80.000	82.1	10.000	52.4	2.000	17.9		
70.000	80.2	9.000	50.6	1.000	7.6		
60.000	77.9	8.000	48.6	0.900	6.4		



Micromeritics Instrument Corporation

Saturn DigiSizer 5200 V1.12

Saturn DigiSizer 5200 V1.12

5200 LSHU V2.01 S/N 216

Page 3

Sample: T2IS1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-953.SMP

Test Number: 3
Analyzed: 2026/06/18 11:45:44PM
Reported: 2026/06/29 9:30:43PM
Background: 2026/06/18 10:38:57PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.7%

Report by Volume Percent


Low Diameter (μm)	Cumulative Volume Finer (Percent)	Low Diameter (μm)	Cumulative Volume Finer (Percent)	Low Diameter (μm)	Cumulative Volume Finer (Percent)
134.359	90.0	8.677	50.0	1.234	10.0

Sample: T2IS1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-953.SMP

Test Number: 3
Analyzed: 2026/06/18 11:45:44PM
Reported: 2026/06/29 9:30:43PM
Background: 2026/06/18 10:38:57PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.7%

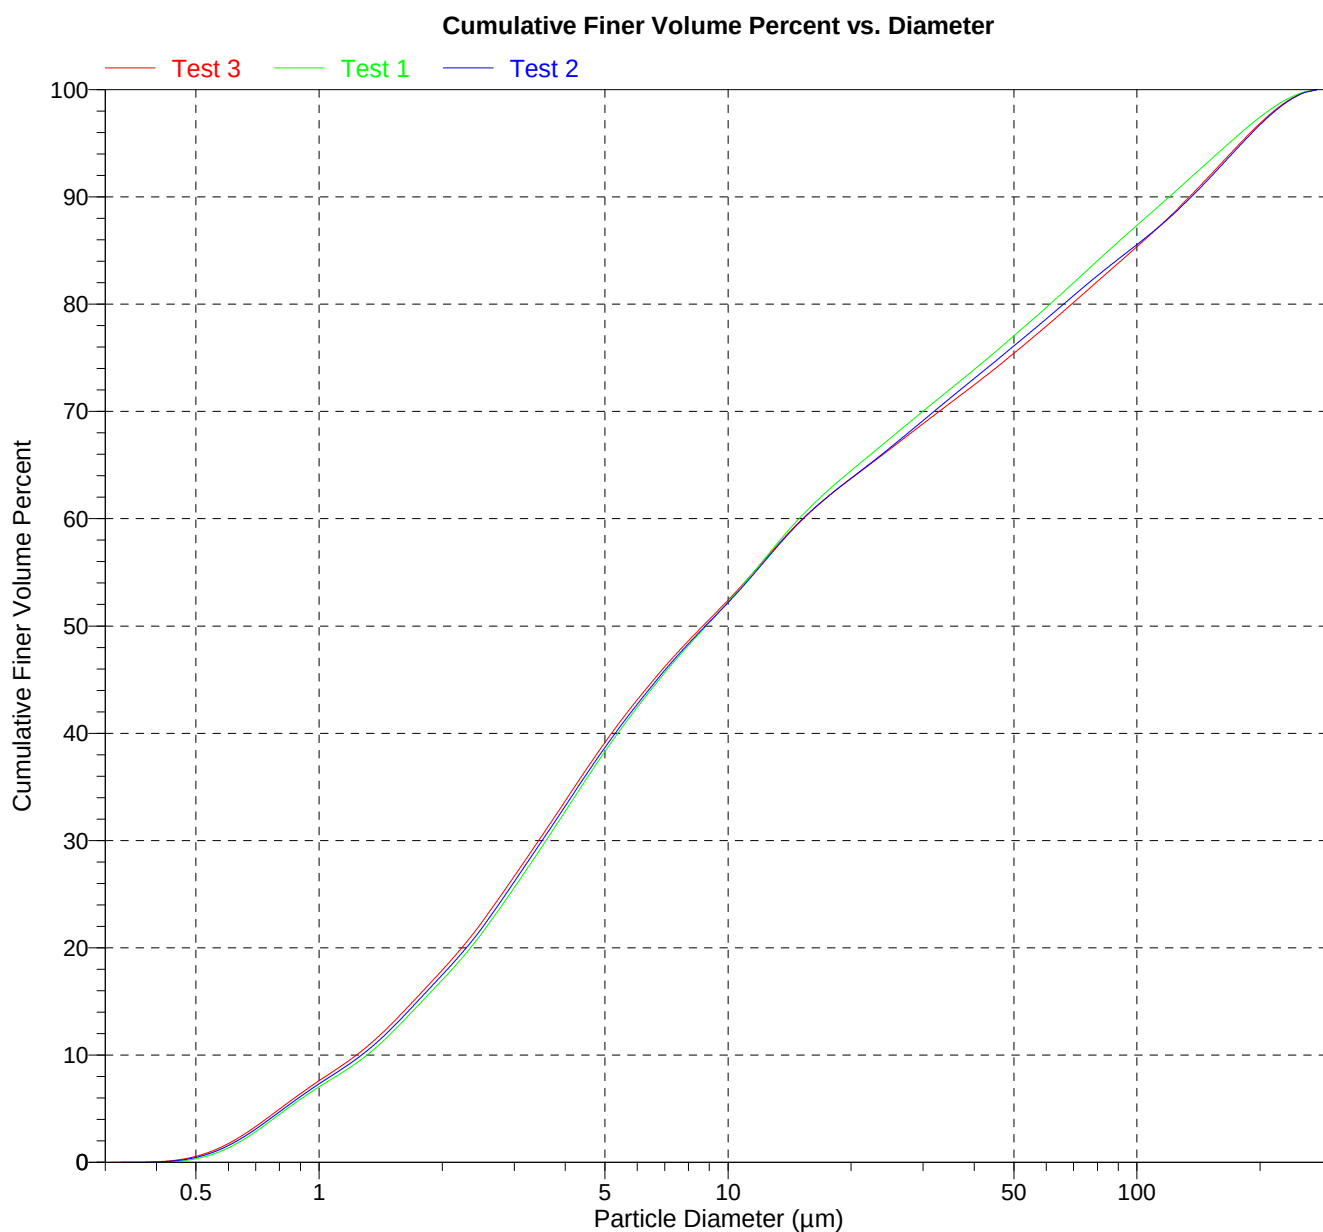


Sample: T2IS1
 Operator: LvdM, ChemEng, Stb Uni
 Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
 File: C:\...\RHASCH~1\005-953.SMP

Test Number: 3
 Analyzed: 2026/06/18 11:45:44PM
 Reported: 2026/06/29 9:30:43PM
 Background: 2026/06/18 10:38:57PM

Model: (1.520, 0.1000000), 1.331
 Material: Sand / Water
 Background: Water RI 1.331
 Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.7%

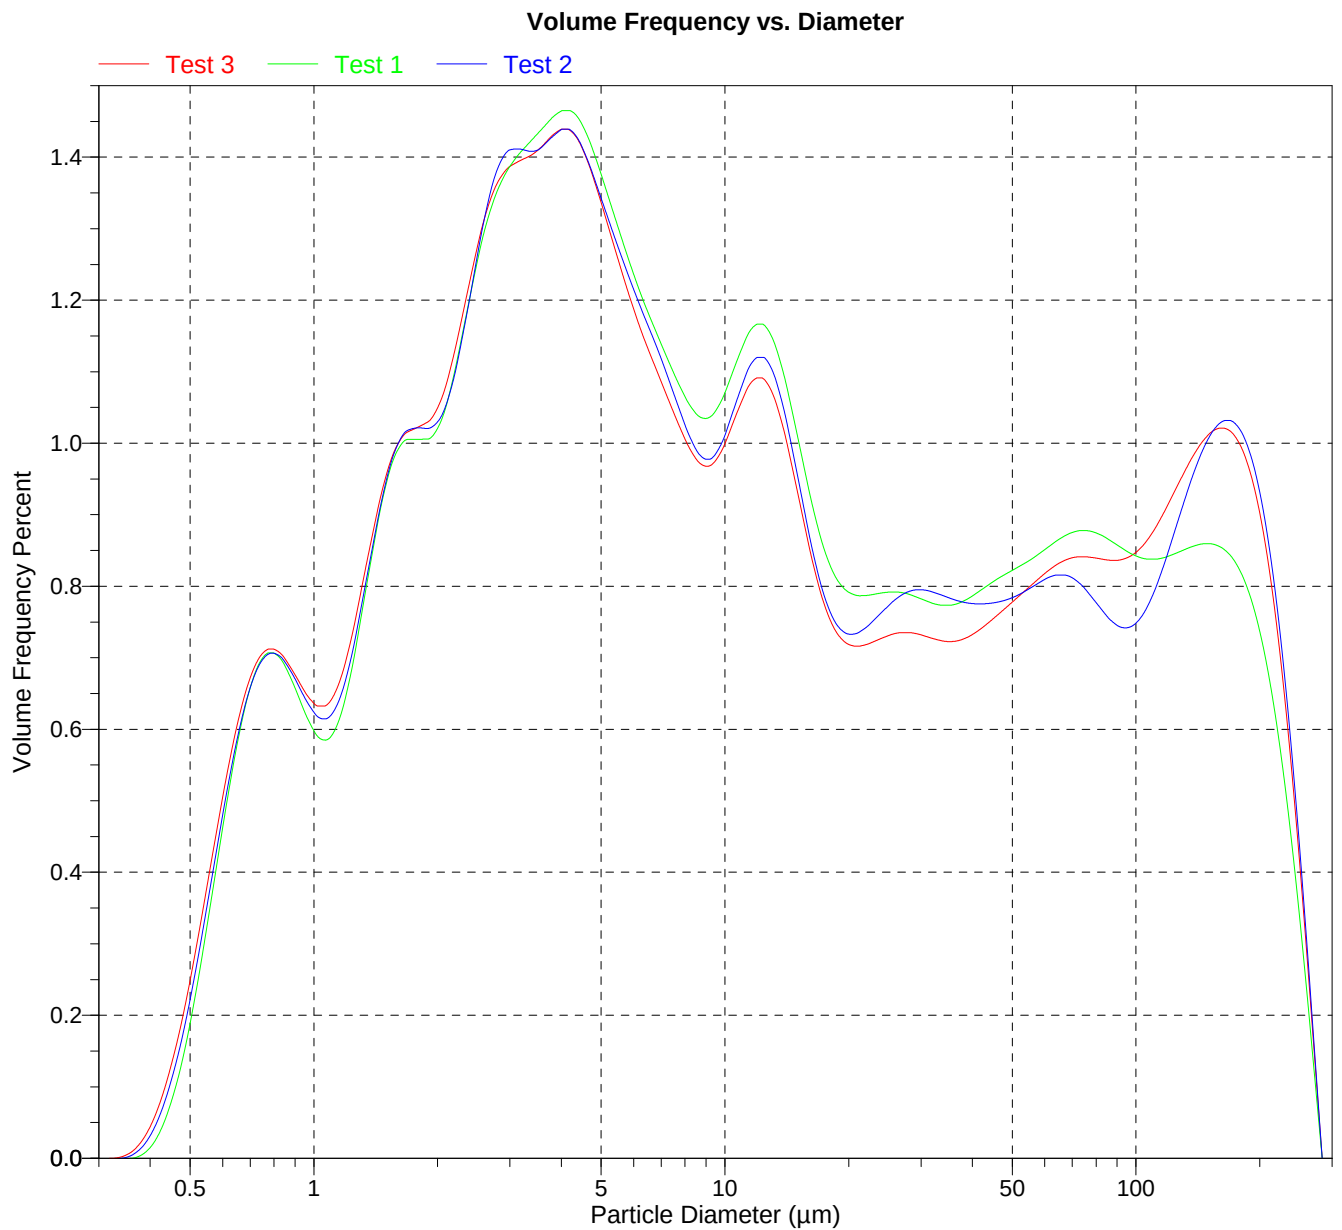

Sample: T2IS1
 Operator: LvdM, ChemEng, Stb Uni
 Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
 File: C:\...\RHASCH~1\005-953.SMP

Test Number: 3
 Analyzed: 2026/06/18 11:45:44PM
 Reported: 2026/06/29 9:30:43PM
 Background: 2026/06/18 10:38:57PM

Model: (1.520, 0.1000000), 1.331
 Material: Sand / Water
 Background: Water RI 1.331
 Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.7%

