


Sample: T2SG1
 Operator: LvdM, ChemEng, Stb Uni
 Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
 File: C:\...\RHASCH~1\005-950.SMP

Test Number: 3
 Analyzed: 2026/06/17 15:37:17PM
 Reported: 2026/06/29 9:27:14PM
 Background: 2026/06/17 10:31:40PM

Model: (1.520, 0.1000000), 1.331
 Material: Sand / Water
 Background: Water RI 1.331
 Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 11.0%

Combined Report

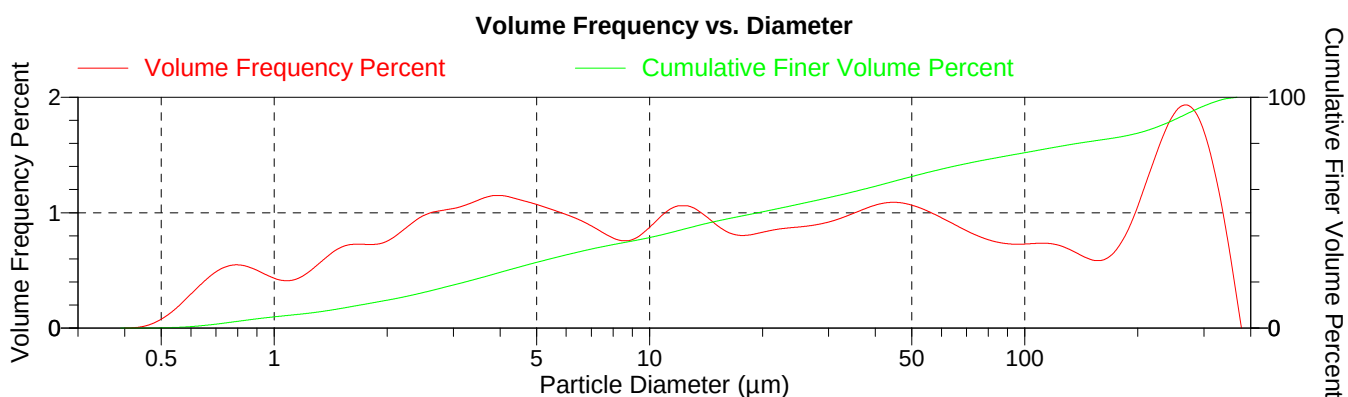

Summary Report

Analysis Conditions

FlowRate: 12.0 l/m
 Circulation time: 60 sec

Ultrasonic intensity: 60 %
 Ultrasonic time: 75 sec

Sample

Sample Concentration: 0.00554 %
 Obscuration: 14.6 %

Volume Distribution Arithmetic Statistics

		Std Dev of 3			Std Dev of 3
Mean	69.47	4.484	Mode	267.7	0.000
Median	19.50	3.302			

Selected Sizes

Diameter (µm)	Percent Finer
100.0	76.0
50.00	65.7
20.00	50.4
10.00	39.2
1.000	4.9

Peaks

Peak Number	% of Dist.*	% of Dist. Std Dev of 3	Mean	Mean Std Dev of 3	Median	Median Std Dev of 3	Mode
1	5.5	N/A	0.793	N/A	0.786	N/A	0.799
2	5.5	N/A	1.475	N/A	1.478	N/A	1.689
3	26.3	N/A	4.373	N/A	4.004	N/A	4.005
4	11.9	N/A	12.92	N/A	12.61	N/A	11.96
5	26.5	N/A	46.51	N/A	42.16	N/A	44.94
6	6.1	N/A	126.5	N/A	124.3	N/A	112.9
7	18.2	N/A	256.3	N/A	255.1	N/A	267.7

* Peaks must comprise at least 5.00 % of the distribution.

Sample: T2SG1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-950.SMP

Test Number: 3
Analyzed: 2026/06/17 15:37:17PM
Reported: 2026/06/29 9:27:14PM
Background: 2026/06/17 10:31:40PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 11.0%

Report by Size Table

Low Diameter (μm)	Cumulative Volume Finer (Percent)	Low Diameter (μm)	Cumulative Volume Finer (Percent)	Low Diameter (μm)	Cumulative Volume Finer (Percent)	Low Diameter (μm)	Cumulative Volume Finer (Percent)
300.000	96.2	60.000	68.9	8.000	36.2	0.900	4.0
250.000	90.2	50.000	65.7	7.000	34.2	0.800	2.9
200.000	84.5	40.000	61.5	6.000	31.7	0.700	1.7
150.000	80.9	30.000	56.5	5.000	28.5	0.600	0.6
100.000	76.0	25.000	53.7	4.000	24.1	0.500	0.1
90.000	74.7	20.000	50.4	3.000	18.6		
80.000	73.1	10.000	39.2	2.000	12.1		
70.000	71.3	9.000	37.7	1.000	4.9		



Micromeritics Instrument Corporation

Saturn DigiSizer 5200 V1.12

Saturn DigiSizer 5200 V1.12

5200 LSHU V2.01 S/N 216

Page 3

Sample: T2SG1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-950.SMP

Test Number: 3
Analyzed: 2026/06/17 15:37:17PM
Reported: 2026/06/29 9:27:14PM
Background: 2026/06/17 10:31:40PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 11.0%

Report by Volume Percent


Low Diameter (μm)	Cumulative Volume Finer (Percent)	Low Diameter (μm)	Cumulative Volume Finer (Percent)	Low Diameter (μm)	Cumulative Volume Finer (Percent)
248.106	90.0	19.503	50.0	1.696	10.0

Sample: T2SG1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-950.SMP

Test Number: 3
Analyzed: 2026/06/17 15:37:17PM
Reported: 2026/06/29 9:27:14PM
Background: 2026/06/17 10:31:40PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 11.0%

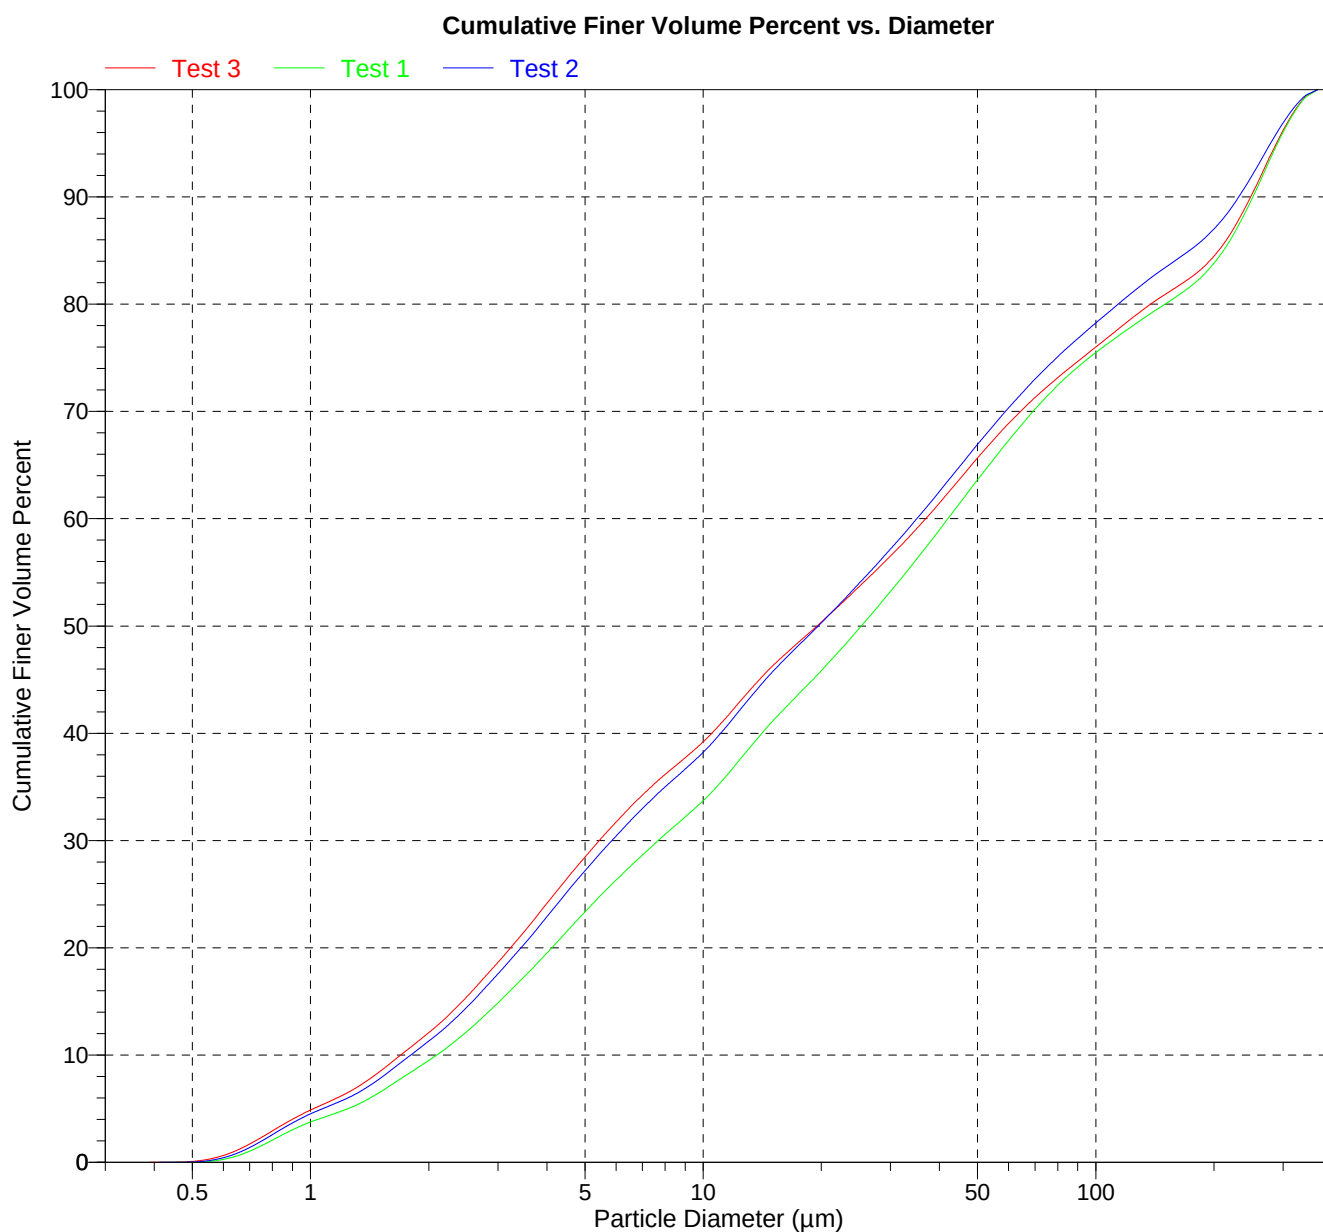


Sample: T2SG1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-950.SMP

Test Number: 3
Analyzed: 2026/06/17 15:37:17PM
Reported: 2026/06/29 9:27:14PM
Background: 2026/06/17 10:31:40PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 11.0%

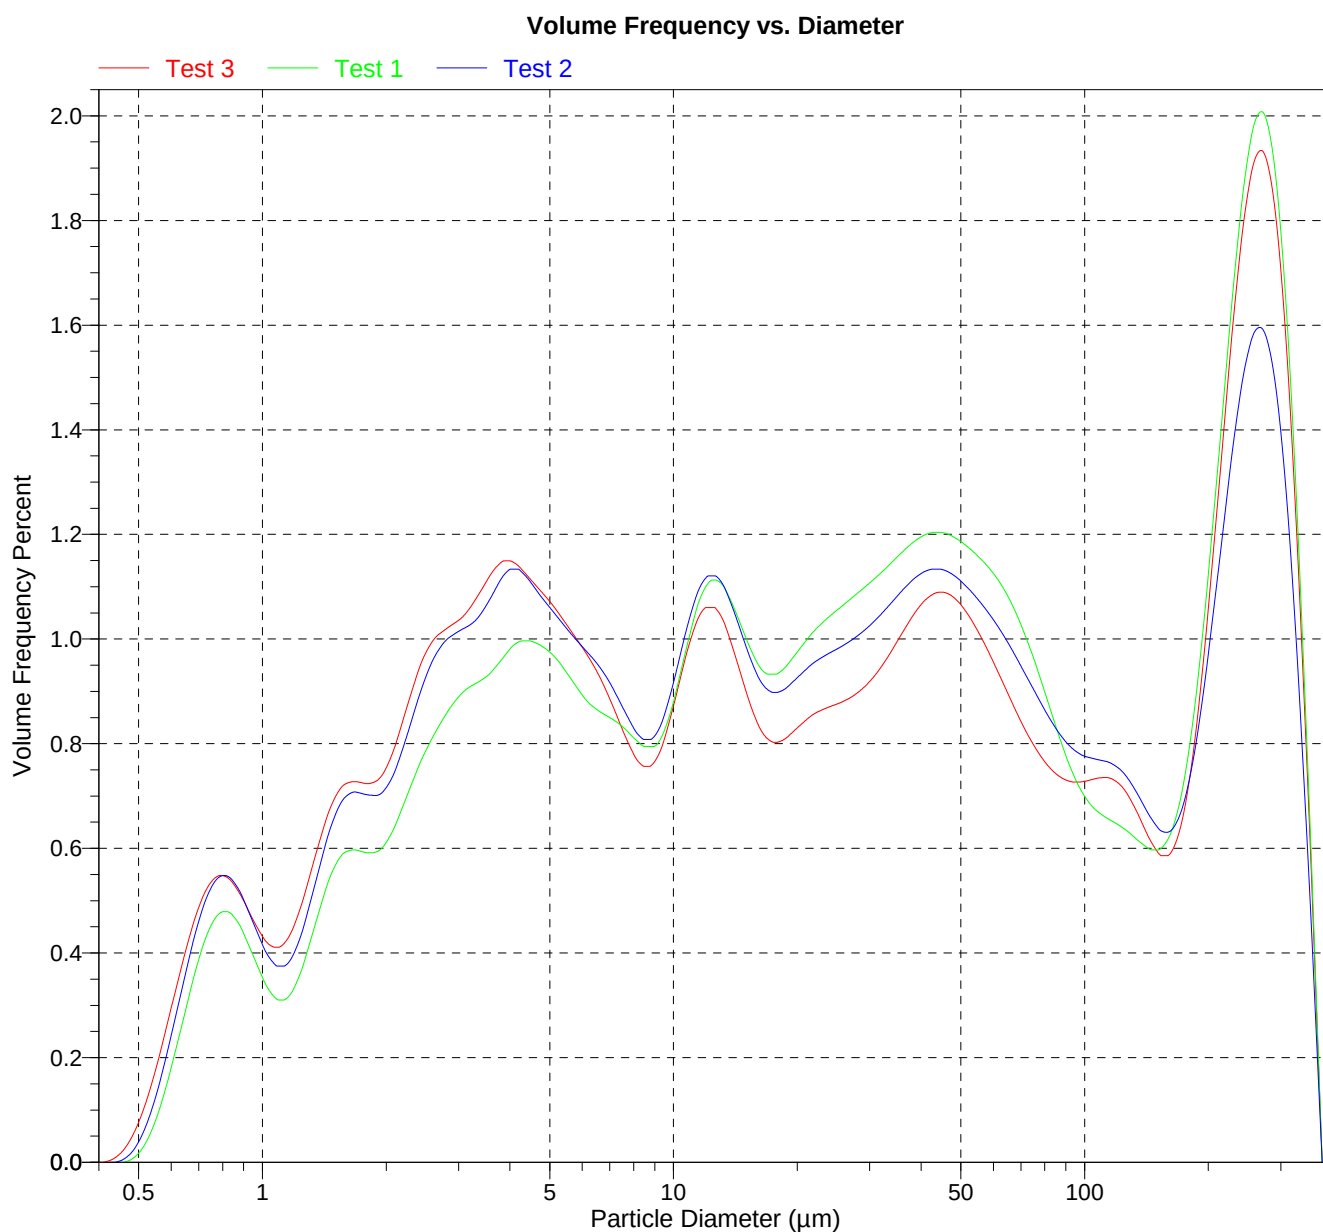

Sample: T2SG1
Operator: LvdM, ChemEng, Stb Uni
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu
File: C:\...\RHASCH~1\005-950.SMP

Test Number: 3
Analyzed: 2026/06/17 15:37:17PM
Reported: 2026/06/29 9:27:14PM
Background: 2026/06/17 10:31:40PM

Model: (1.520, 0.1000000), 1.331
Material: Sand / Water
Background: Water RI 1.331
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 11.0%

