


Sample: T3IS1  
 Operator: LvdM, ChemEng, Stb Uni  
 Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu  
 File: C:\...\RHASCH~1\005-962.SMP

Test Number: 3  
 Analyzed: 2026/06/26 10:50:17PM  
 Reported: 2026/06/29 11:06:47PM  
 Background: 2026/06/26 9:53:13PM

Model: (1.520, 0.1000000), 1.331  
 Material: Sand / Water  
 Background: Water RI 1.331  
 Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.5%

### Combined Report

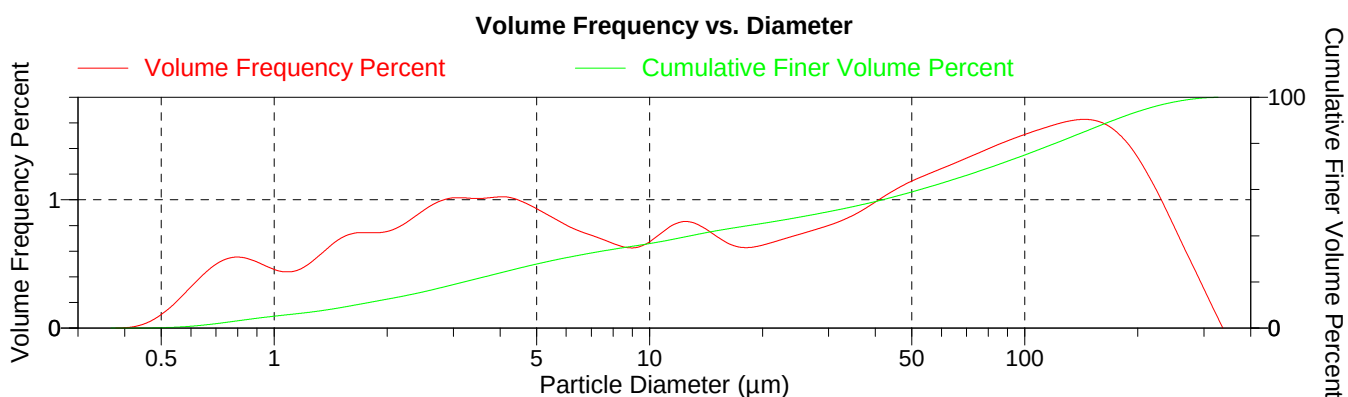

### Summary Report

#### Analysis Conditions

FlowRate: 12.0 l/m  
 Circulation time: 60 sec

Ultrasonic intensity: 60 %  
 Ultrasonic time: 75 sec

#### Sample

Sample Concentration: 0.00434 %  
 Obscuration: 11.4 %

#### Volume Distribution Arithmetic Statistics

|        |       |              |      |       |              |
|--------|-------|--------------|------|-------|--------------|
|        |       | Std Dev of 3 |      |       | Std Dev of 3 |
| Mean   | 60.79 | 0.722        | Mode | 142.1 | 23.57        |
| Median | 29.07 | 0.463        |      |       |              |

#### Selected Sizes

| Diameter (µm) | Percent Finer |
|---------------|---------------|
| 100.0         | 75.0          |
| 50.00         | 59.0          |
| 20.00         | 45.3          |
| 10.00         | 36.6          |
| 1.000         | 5.2           |

#### Peaks

| Peak Number | % of Dist.* | % of Dist. Std Dev of 3 | Mean  | Mean Std Dev of 3 | Median | Median Std Dev of 3 | Mode  |
|-------------|-------------|-------------------------|-------|-------------------|--------|---------------------|-------|
| 1           | 5.9         | N/A                     | 0.787 | N/A               | 0.781  | N/A                 | 0.799 |
| 2           | 6.3         | N/A                     | 1.523 | N/A               | 1.524  | N/A                 | 1.789 |
| 3           | 10.2        | N/A                     | 2.768 | N/A               | 2.749  | N/A                 | 3.182 |
| 4           | 13.3        | N/A                     | 5.764 | N/A               | 5.434  | N/A                 | 4.005 |
| 5           | 8.7         | N/A                     | 13.21 | N/A               | 12.92  | N/A                 | 12.67 |
| 6           | 55.6        | N/A                     | 105.2 | N/A               | 89.71  | N/A                 | 142.1 |

\* Peaks must comprise at least 5.00 % of the distribution.

Sample: T3IS1  
Operator: LvdM, ChemEng, Stb Uni  
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu  
File: C:\...\RHASCH~1\005-962.SMP

Test Number: 3  
Analyzed: 2026/06/26 10:50:17PM  
Reported: 2026/06/29 11:06:47PM  
Background: 2026/06/26 9:53:13PM

Model: (1.520, 0.1000000), 1.331  
Material: Sand / Water  
Background: Water RI 1.331  
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.5%

**Report by Size Table**

| Low<br>Diameter<br>( $\mu$ m) | Cumulative<br>Volume<br>Finer<br>(Percent) | Low<br>Diameter<br>( $\mu$ m) | Cumulative<br>Volume<br>Finer<br>(Percent) | Low<br>Diameter<br>( $\mu$ m) | Cumulative<br>Volume<br>Finer<br>(Percent) | Low<br>Diameter<br>( $\mu$ m) | Cumulative<br>Volume<br>Finer<br>(Percent) |
|-------------------------------|--------------------------------------------|-------------------------------|--------------------------------------------|-------------------------------|--------------------------------------------|-------------------------------|--------------------------------------------|
| 300.000                       | 99.7                                       | 60.000                        | 62.8                                       | 8.000                         | 34.1                                       | 0.900                         | 4.3                                        |
| 250.000                       | 98.0                                       | 50.000                        | 59.0                                       | 7.000                         | 32.5                                       | 0.800                         | 3.2                                        |
| 200.000                       | 93.8                                       | 40.000                        | 54.8                                       | 6.000                         | 30.5                                       | 0.700                         | 1.9                                        |
| 150.000                       | 86.2                                       | 30.000                        | 50.4                                       | 5.000                         | 27.7                                       | 0.600                         | 0.8                                        |
| 100.000                       | 75.0                                       | 25.000                        | 48.0                                       | 4.000                         | 23.9                                       | 0.500                         | 0.1                                        |
| 90.000                        | 72.3                                       | 20.000                        | 45.3                                       | 3.000                         | 18.8                                       | 0.400                         | 0.0                                        |
| 80.000                        | 69.4                                       | 10.000                        | 36.6                                       | 2.000                         | 12.5                                       |                               |                                            |
| 70.000                        | 66.2                                       | 9.000                         | 35.4                                       | 1.000                         | 5.2                                        |                               |                                            |



**Micromeritics Instrument Corporation**

Saturn DigiSizer 5200 V1.12

Saturn DigiSizer 5200 V1.12

5200 LSHU V2.01 S/N 216

Page 3

Sample: T3IS1  
Operator: LvdM, ChemEng, Stb Uni  
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu  
File: C:\...\RHASCH~1\005-962.SMP

Test Number: 3  
Analyzed: 2026/06/26 10:50:17PM  
Reported: 2026/06/29 11:06:47PM  
Background: 2026/06/26 9:53:13PM

Model: (1.520, 0.1000000), 1.331  
Material: Sand / Water  
Background: Water RI 1.331  
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.5%

**Report by Volume Percent**


| Low<br>Diameter<br>( $\mu\text{m}$ ) | Cumulative<br>Volume<br>Finer<br>(Percent) | Low<br>Diameter<br>( $\mu\text{m}$ ) | Cumulative<br>Volume<br>Finer<br>(Percent) | Low<br>Diameter<br>( $\mu\text{m}$ ) | Cumulative<br>Volume<br>Finer<br>(Percent) |
|--------------------------------------|--------------------------------------------|--------------------------------------|--------------------------------------------|--------------------------------------|--------------------------------------------|
| 172.084                              | 90.0                                       | 29.066                               | 50.0                                       | 1.645                                | 10.0                                       |

Sample: T3IS1  
Operator: LvdM, ChemEng, Stb Uni  
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu  
File: C:\...\RHASCH~1\005-962.SMP

Test Number: 3  
Analyzed: 2026/06/26 10:50:17PM  
Reported: 2026/06/29 11:06:47PM  
Background: 2026/06/26 9:53:13PM

Model: (1.520, 0.1000000), 1.331  
Material: Sand / Water  
Background: Water RI 1.331  
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.5%

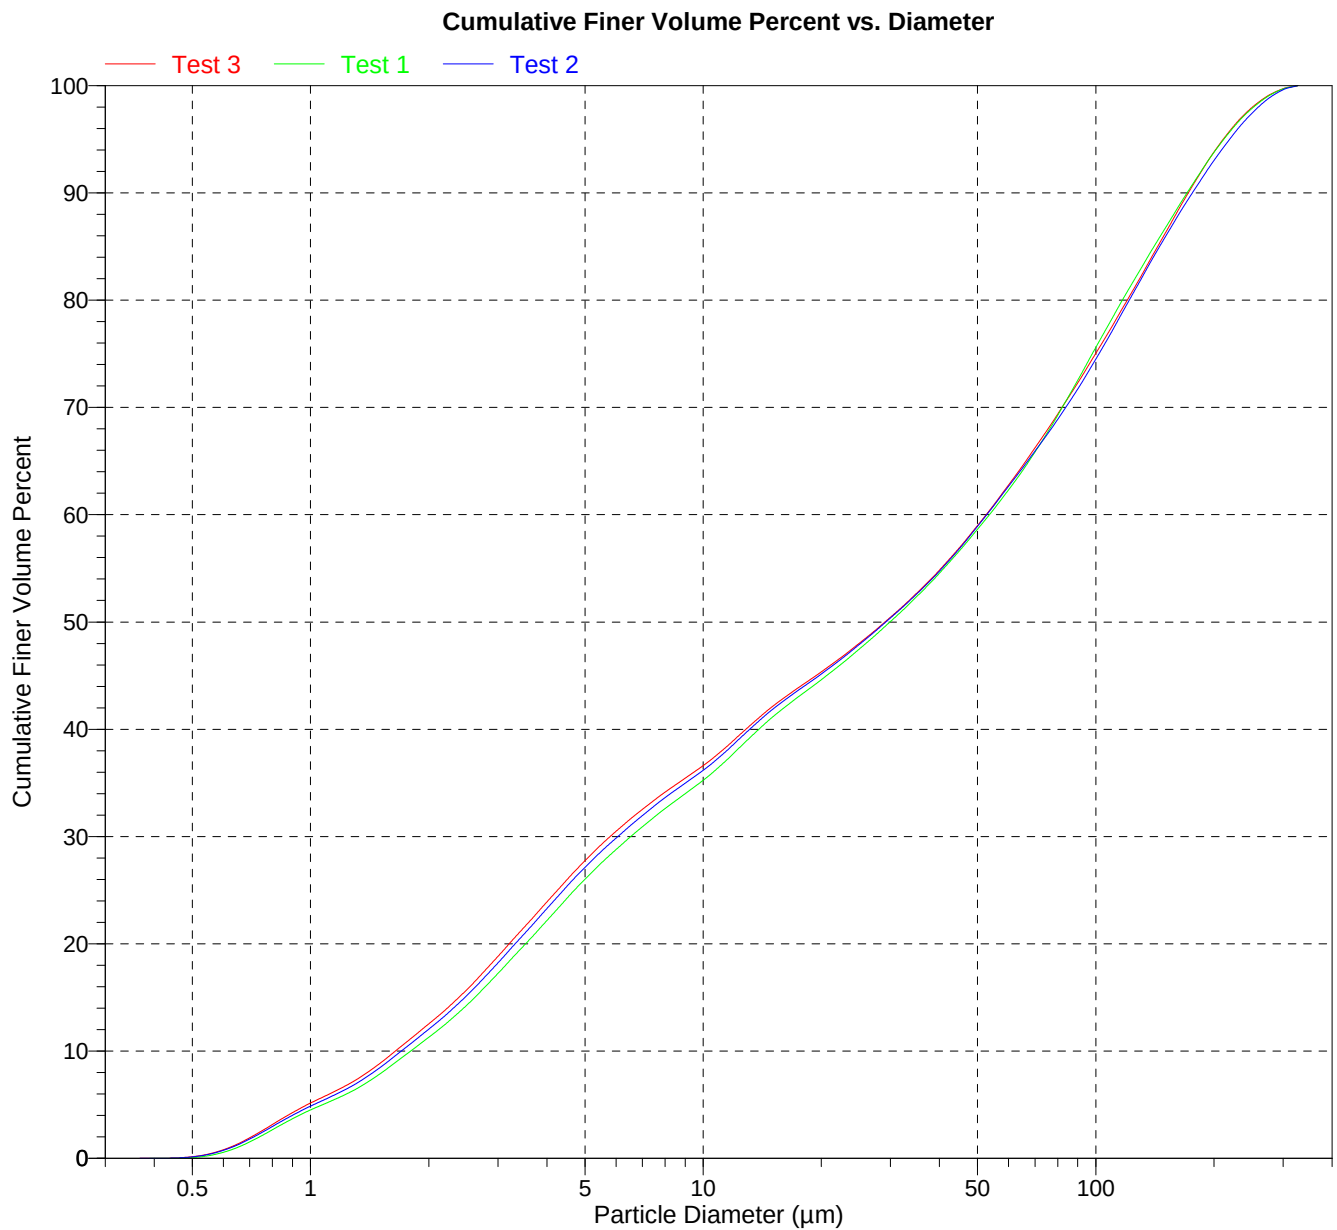


Sample: T3IS1  
Operator: LvdM, ChemEng, Stb Uni  
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu  
File: C:\...\RHASCH~1\005-962.SMP

Test Number: 3  
Analyzed: 2026/06/26 10:50:17PM  
Reported: 2026/06/29 11:06:47PM  
Background: 2026/06/26 9:53:13PM

Model: (1.520, 0.1000000), 1.331  
Material: Sand / Water  
Background: Water RI 1.331  
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.5%

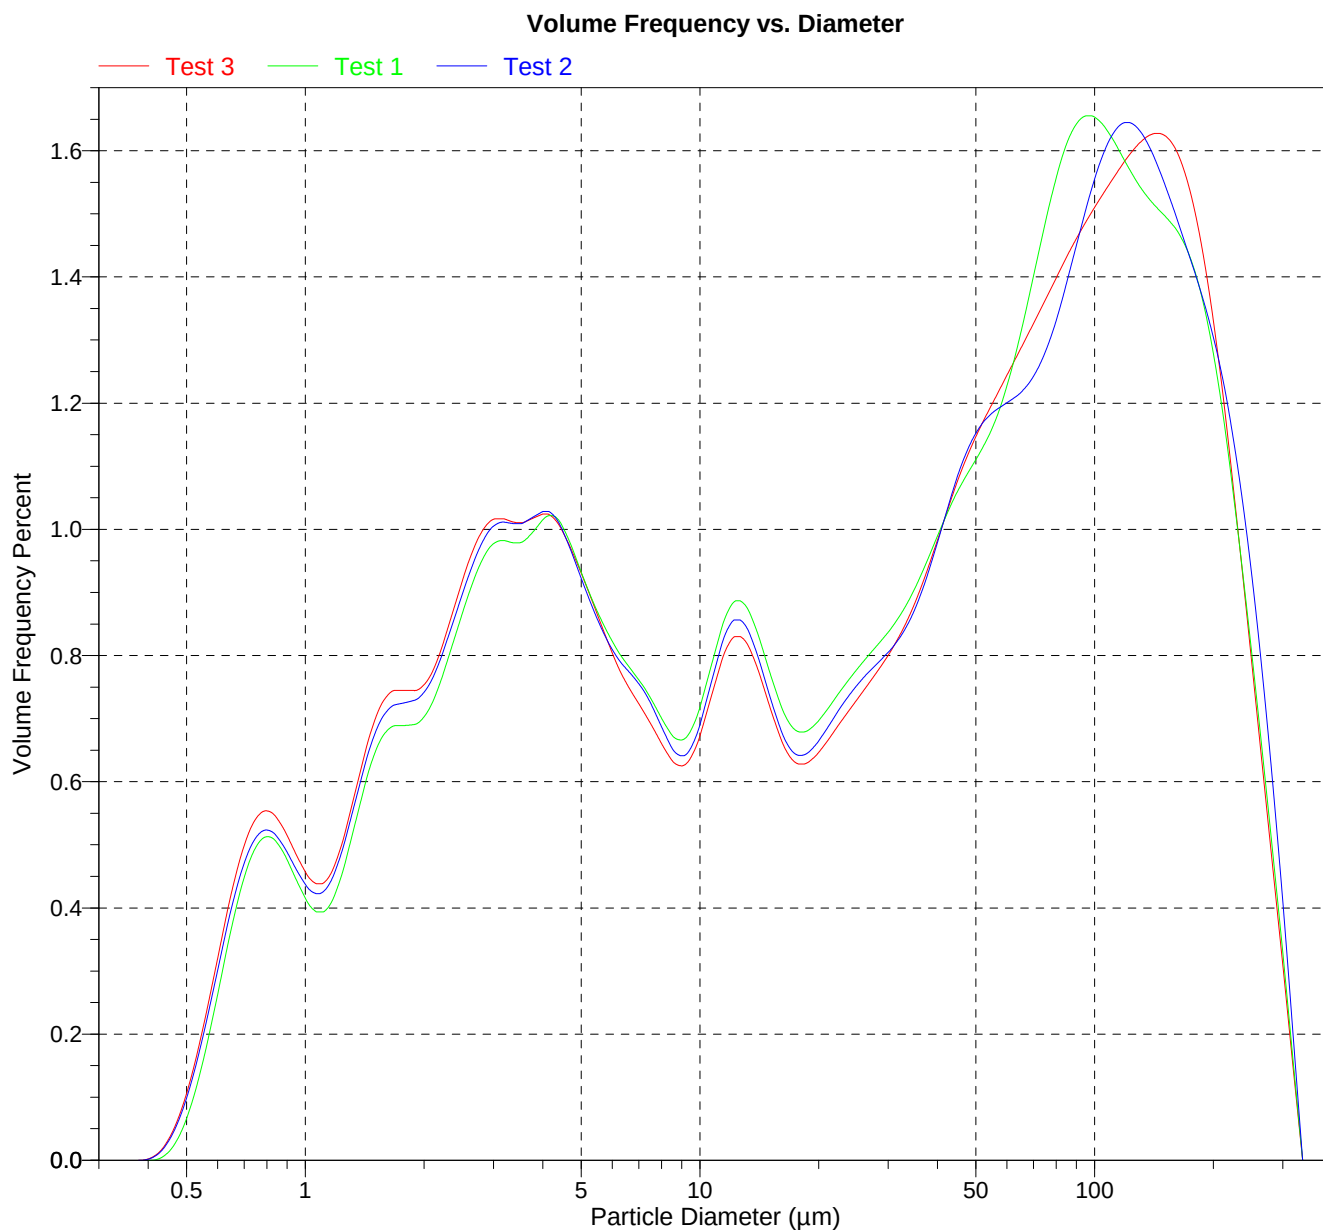

Sample: T3IS1  
Operator: LvdM, ChemEng, Stb Uni  
Submitter: Rebekah Haschick, BotZoo, Dr Ndlovu  
File: C:\...\RHASCH~1\005-962.SMP

Test Number: 3  
Analyzed: 2026/06/26 10:50:17PM  
Reported: 2026/06/29 11:06:47PM  
Background: 2026/06/26 9:53:13PM

Model: (1.520, 0.1000000), 1.331  
Material: Sand / Water  
Background: Water RI 1.331  
Smoothing: Medium

Comments: 0.0005% TSPP. Initial obsc = 10.5%

