Glucose Twin

Digital health • ML • Streamlit

How the project works — from glucose readings to a 2-hour risk estimate

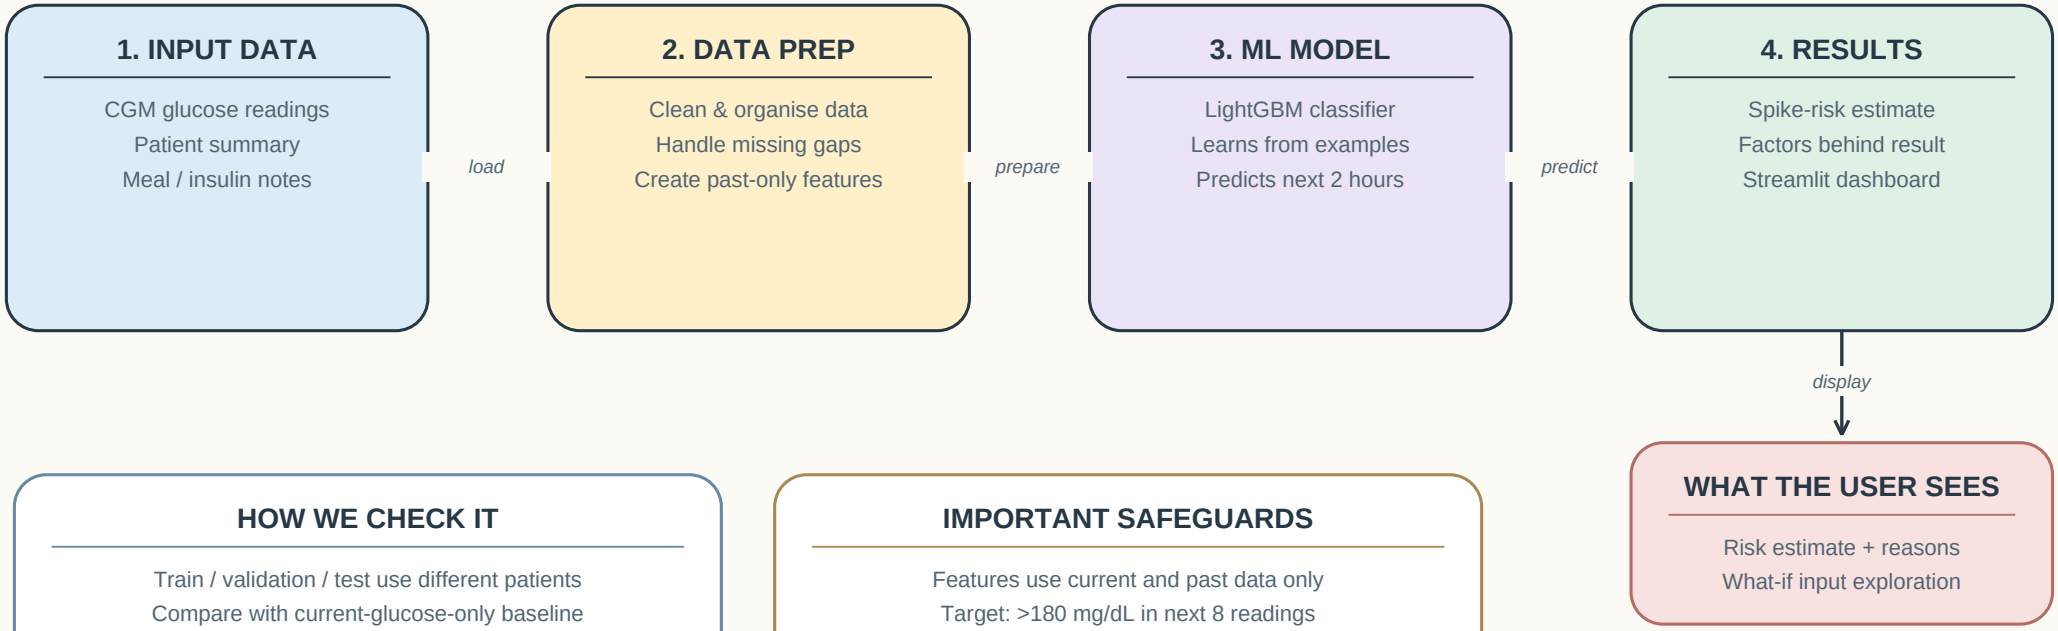

HOW WE CHECK IT

Train / validation / test use different patients
Compare with current-glucose-only baseline
Report PR-AUC, ROC-AUC, precision, recall and F1

IMPORTANT SAFEGUARDS

Features use current and past data only
Target: >180 mg/dL in next 8 readings
Each reading is about 15 minutes apart

PLEASE REMEMBER

Research prototype only — not a medical device or a substitute for clinical advice.
Real-data performance must be measured; synthetic data is only for testing the app.