



2015 -2016 PRODUCT CATALOGUE

Broche[®]
Medical

ABOUT US

Nurteks Tekstil Nakış San. ve Tic. Ltd. Şti. has started production and sale of disposable surgical gowns and surgical drape sets with **Broche®** brand in its own facilities in the beginning of 2006 to convey its experiment, in non-woven sector since 1995, to medical sector.

Nurteks Tekstil, having a well earned place in all over Turkey with **Broche®** brand by quick delivering all kinds of consumable goods, mostly gloves, which have been produced and, as well, imported since its establishment, 2006, has hold a prominent place and been an important brand, especially, in the markets of Europe, Africa and Middle East with its export activities.

Nurteks Tekstil, making use of ever developing technologies since the beginning of 2012, improved its all machine lines and sterilization devices, and extended its production and stock areas to a total 7.000 SM closed area.

Nurteks Tekstil is steadily carrying on its activities to hold the prominence to be one of the leading brands in the medical sector with high quality and fair price it has been offering in the market with **Broche®** brand.

Quality Policy;

- To make production in the medical sector with the latest technology and provide persistence in production quality and a quality management system.
- To enhance the customer satisfaction by taking any suggestions and complaints into consideration.
- To offer products and services in compliance with current laws and regulations by giving due importance to human health.

Certificates;

CE2195, ISO 13485, ISO 9001,

All drapes and gowns are

TS EN 13795 + A1 certified by TURKISH STANDARDS INSTITUTE.



EN 13795 + A1



INDEX

TEST REPORT

Fabric Test Report 7 - 12

STERILE SURGICAL PACKS

General Surgery Pack - Standard 13
 General Surgery Pack - Large 14
 General Surgery Pack - Extra Large 15
 Laparoscopy Pack 16
 Angiography Pack - Standard 17
 Angiography Pack - Large 18
 Angiography Pack W / Transparent Panel Standard 19
 Angiography Pack W / Transparent Panel Large 20
 Cardiovascular Pack W / Pouch - Standard 21
 Cardiovascular Pack W / Pouch - Large 22
 Tur Pack W \ Pouch (Urology Set) 23
 Lithotomic Gynaecology Pack W / Pouch 24
 Gynaecology / Cystoscopy Pack 25
 Caesarean Section Pack W / Pouch - Standard 26
 Caesarean Section Pack W / Pouch - Large 27
 Caesarean Section Pack W / Pouch - Extra Large 28
 Delivery Pack 29
 Delivery Pack W / Pouch 30
 Arthroscopy Pack W / Pouch - Standard 31
 Arthroscopy Pack W / Pouch - Large 32
 Arthroscopy Pack W / Pouch - Extra Large 33
 Craniotomy W / Pouch Pack 34
 E.N.T. Pack 35
 Hip Pack U 36
 Implant Pack 37
 Single Pouch Ophthalmic Pack 38
 Adhesive Drapes 39
 Non Sterile Welcome Pack (Waterproof) 40

STERILE PROCEDURE PACKS

Major General Procedure Pack 44
 Cardiology-Angiography Procedure Pack 46
 Caesarean Procedure Pack 48
 Open Heart CABG Procedure Pack 50
 Gynaecology Procedure Pack 52
 Urology Procedure Pack 54
 Orthopedic Hip Replacement Procedure Pack 56
 Orthopaedic Knee Arthroscopy Procedure Pack 58
 Cataract Procedure Pack 60

STERILE & NON-STERILE GOWNS

Sterile Ultrasonic Stitch Surgical Gown 64
 Non-Sterile Patient Gown 66
 Non-Sterile Doctor Scrub Suit 66

GLOVES

Chloroprene Synthetic Sterile Surgical Gloves 69
 Latex Sterile Surgical Gloves 70
 Latex Examination Gloves - Powdered 71
 Latex Examination Gloves - Powder Free 72
 Vinyl Examination Gloves - Powdered 73
 Vinyl Examination Gloves - Powder Free 74
 Nitrile Examination Gloves 75
 Nitrile Chemotherapy Examination Gloves 76
 Pe Gloves 77

STERILE PLASTIC PRODUCTS


Flowmeter 79
 Infusion (Serum) Set 79
 Urine Bag / T-Value and Push & Pull Valve 80
 Blood Transfusion Set 81

MEDICAL DISPOSABLES

Steril Surgical Blades 83
 Blood Lancet 84
 Wooden Tongue Depressor 85
 Shoe Covers 86
 Face Mask 87
 Soft Bar Cap 88

CERTIFICATES

Certificates 89 - 92

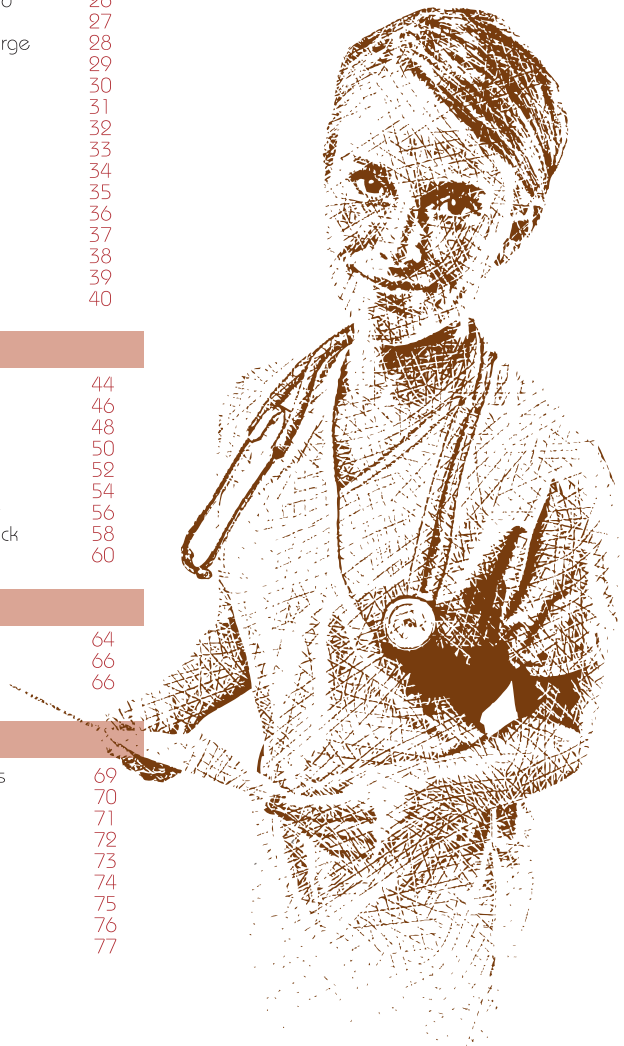

EN 13795


European Standard for Surgical Drapes and Gowns

Introduction

This document provides an overview of the EN 13795 European Standard for surgical gowns and drapes, which outlines their performance requirements, test methodologies and explains the overall relevance to patients and the clinical staff.

The broad aim of EN 13795 is to establish an European recognised standard of quality and conformance to manufacturing, testing and performance specifications for all single-use and multiple-use surgical drapes and gowns.

Key aspects of Section 6



General requirements for Manufacturers, Processors and Products

Compliance with this Standard demonstrates that the device is fit for purpose and can be used on a patient as it conforms to a range of relevant testing procedures. This information must be fulfilled by the manufacturers and processors and all test methods and results must be made available as part of a quality assurance system, for both single-use and reusable devices.

It should be noted that surgical drapes and gowns are further categorised according to their performance and defined as **standard** or **high performance** devices.

General requirements

The manufacturer or processor must:

- for reusable devices: provide information on the appropriate process to allow re-use (cleaning, disinfection, packaging, sterilisation methods) including number of re-uses and any restriction to the re-use
- for sterile devices: provide instructions for sterilization methods
- differentiate between critical and less critical areas on the device, where appropriate, as well as physical identification of these areas
- upon request, reference test methods used, and corresponding test results (see Tables 1, 2, and 3), differentiating critical and less critical areas with appropriate rationale for the differentiation
- use validated manufacturing and processing procedures

General product requirements:

- it shall be possible to demonstrate that the product requirements of EN 13795 are met (see Tables 4, 5 and 6), and test results shall be recorded and retained
- the finished product (after sterilisation if appropriate) shall be tested prior to commercialisation
- during manufacturing and processing, testing shall be done according to the requirements of the manufacturer's or processor's quality system




Key aspects of Annex B

Test Methods

EN 13795 describes the standardised and harmonised test methodologies that all single-use and reusable surgical drapes, gowns and clean air suits must undergo, as part of a quality assurance system.

Test of resistance to microbial dry penetration - EN ISO 22612

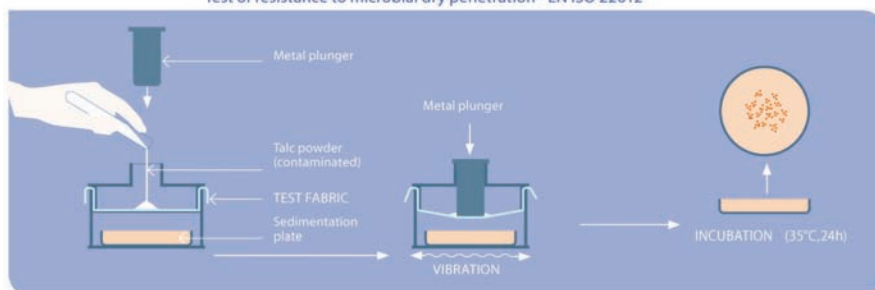

The test method is designed to determine the ability of materials to resist penetration of particles carrying micro-organisms under dry fabric conditions.

The method establishes the quantity of micro-organisms that can penetrate through the test material being carried on talcum powder.

Test results are expressed in CFU (colony forming units) that were observed on the agar plate.

Table 1 - Performance requirements for microbial dry penetration

Unit	Surgical Gowns				Surgical Drapes			
	Standard Performance		High Performance		Standard Performance		High Performance	
	critical area	less critical area	critical area	less critical area	critical area	less critical area	critical area	less critical area
CFU	N/A	≤ 300 ^a	N/A	≤ 300 ^a	N/A	≤ 300 ^a	N/A	≤ 300 ^a

^a Test conditions: challenge concentration 10⁸ CFU/g talc, and 30 minutes vibration time.

Test of resistance to microbial wet penetration - EN ISO 22610



The purpose of this test is to evaluate the ability of fabrics to resist microbial penetration under conditions of liquid pooling on the fabric and mechanical stress. Test results are expressed in I_B "Barrier Index".


Table 2 - Performance requirements for microbial wet penetration

Unit	Surgical Gowns				Surgical Drapes			
	Standard Performance		High Performance		Standard Performance		High Performance	
	critical area	less critical area	critical area	less critical area	critical area	less critical area	critical area	less critical area
I_B	$\geq 2,8^b$	N/A	6,0 ^{b,c}	N/A	$\geq 2,8^b$	N/A	6,0 ^{b,c}	N/A

b The Least Significant Difference (LSD) for I_B when estimated using EN ISO 22610, was found to be 0,98 at the 95% confidence level. This is the minimum difference needed to distinguish between two materials thought to be different. This means materials varying by up to 0,98 I_B are probably not different; materials varying by more than 0,98 I_B probably are different. (The 95% confidence level means that an observer would be correct 19 times out of 20 to accept these alternatives).

c $I_B = 6,0$ for the purpose of this standard means: no penetration. $I_B = 6,0$ is the maximum achievable value.

Test of microbial cleanliness - EN ISO 11737-1

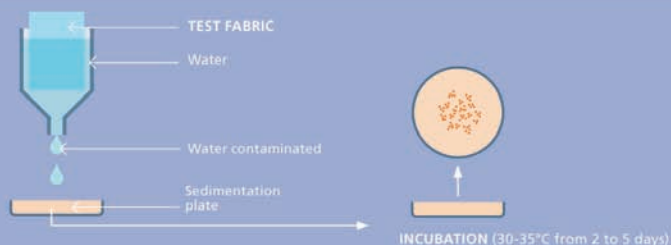

Microbial cleanliness determines the bioburden, meaning the number of viable micro-organisms on the product.

Microbial cleanliness is especially important to achieve sterilisation and a sterilisation assurance level of 10^{-6} as is required to label a product as sterile.

For products that are not sold as sterile, the test method allows assessment of their potential for microbial contamination.

The test results are expressed in a decimal logarithm of CFU/100cm². Lower numbers indicate better cleanliness.

Table 3 - Performance requirements for microbial cleanliness

Unit	Surgical Gowns				Surgical Drapes			
	Standard Performance		High Performance		Standard Performance		High Performance	
	critical area	less critical area	critical area	less critical area	critical area	less critical area	critical area	less critical area
CFU/100 cm ²	≤ 300	≤ 300	≤ 300	≤ 300	≤ 300	≤ 300	≤ 300	≤ 300


Table 5 - Characteristics to be evaluated and Performance Requirements for Surgical Drapes

Performance requirements for Surgical Drapes						
Characteristic	Test method	Unit	Standard Performance		High Performance	
			Critical product area	Less critical product area	Critical product area	Less critical product area
Resistance to microbial penetration – dry	EN ISO 22612	CFU	N/A	≤ 300 ^a	N/A	≤ 300 ^a
Resistance to microbial penetration – wet	EN ISO 22610	I_b	≥ 2,8 ^b	N/A	6,0 ^{b,c}	N/A
Cleanliness – microbial	EN ISO 11737-1	CFU/100 cm ²	≤ 300	≤ 300	≤ 300	≤ 300
Cleanliness – particulate matter	EN ISO 9073-10	IPM	≤ 3,5	≤ 3,5	≤ 3,5	≤ 3,5
Linting	EN ISO 9073-10	log ₁₀ (lint count)	≤ 4,0	≤ 4,0	≤ 4,0	≤ 4,0
Resistance to liquid penetration	EN 20811	cm H ₂ O	≥ 30	≥ 10	≥ 100	≥ 10
Bursting strength – dry	EN ISO 13938-1	kPa	≥ 40	≥ 40	≥ 40	≥ 40
Bursting strength – wet	EN ISO 13938-1	kPa	≥ 40	N/A	≥ 40	N/A
Tensile strength – dry	EN 29073-3	N	≥ 15	≥ 15	≥ 20	≥ 20
Tensile strength – wet	EN 29073-3	N	≥ 15	N/A	≥ 20	N/A

a Test conditions: challenge concentration 10⁶ CFU/g talc. and 30 minutes vibration time.

b The Least Significant Difference (LSD) for I_b when estimated using EN ISO 22610, was found to be 0,98 at the 95% confidence level. This is the minimum difference needed to distinguish between two materials thought to be different. This means materials varying by up to 0,98 I_b are probably not different; materials varying by more than 0,98 I_b probably are different. (The 95% confidence level means that an observer would be correct 19 times out of 20 to accept these alternatives).

c $I_b = 6,0$ for the purpose of this standard means: no penetration. $I_b = 6,0$ is the maximum achievable value.



■ Critical area
■ Less critical area


Table 6 - Characteristics to be evaluated and performance requirements for Clean Air Suits

Performance requirements for Clean Air Suits			
Characteristic	Test method	Unit	Requirement ^a
Resistance to microbial penetration – dry	EN ISO 22612	CFU	≤ 300 ^a
Cleanliness – microbial	EN ISO 11737-1	CFU/100 cm ²	≤ 300
Cleanliness – particulate matter	EN ISO 9073-10	IPM	≤ 3,5
Linting	EN ISO 9073-10	log ₁₀ (lint count)	≤ 4,0
Bursting strength – dry	EN ISO 13938-1	kPa	≥ 40
Tensile strength – dry	EN 29073-3	N	≥ 20

a Test conditions: challenge concentration 10⁶ CFU/g talc. and 30 minutes vibration time.

b Performance requirements apply for all products areas of clean air suits.

General Surgery Pack - Standard

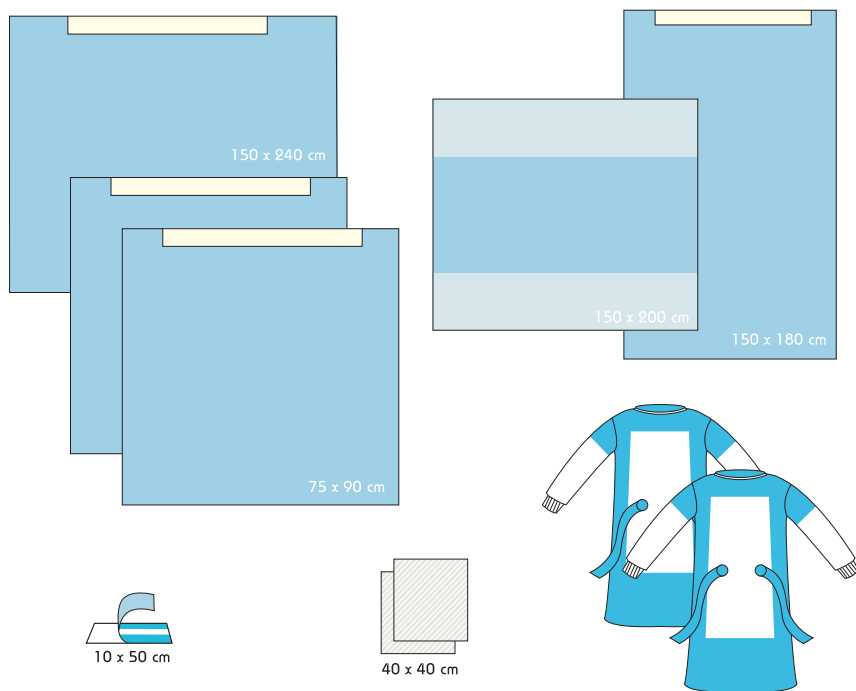

High Absorbent DL
 SMS
 PE Film
 Adhesive Tape


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
ADS009	Anesthesia Drape	150 x 240 cm	1
ADS003	Adhesive Drape	75 x 90 cm	2
ADS008	Adhesive Drape	150 x 180 cm	1
OPS001	Op-Tapes	10 x 50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

GSST001 - NG

*Product contents can be customized upon request

General Surgery Pack - Large

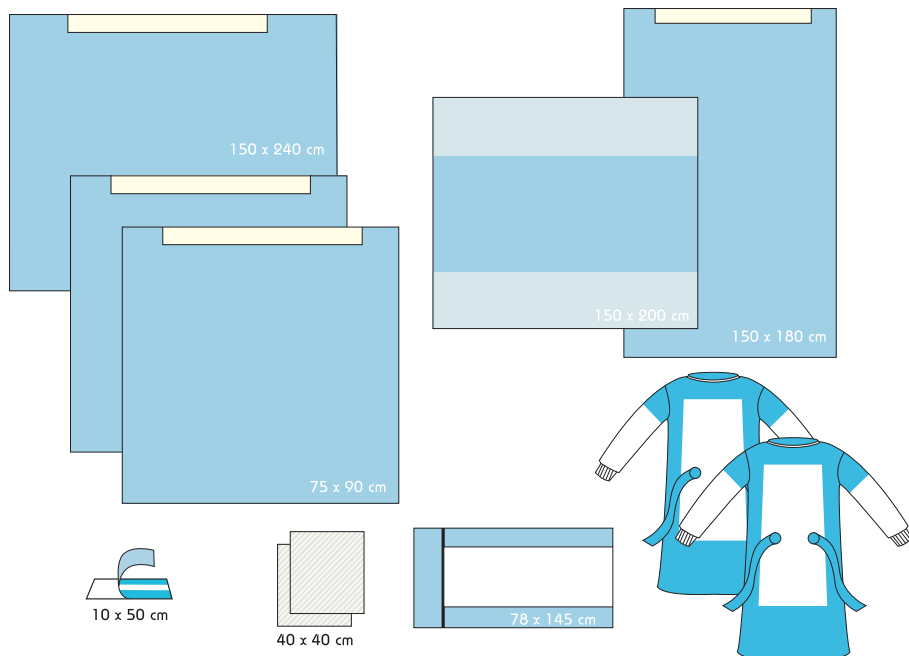

High Absorbent DL
 SMS
 PE Film
 Adhesive Tape


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
ADS009	Anesthesia Drape	150 x 240 cm	1
ADS003	Adhesive Drape	75 x 90 cm	2
ADS008	Adhesive Drape	150 x 180 cm	1
OPS001	Op-Tapes	10 x 50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

GSST002 - NG

*Product contents can be customized upon request

General Surgery Pack - Extra Large

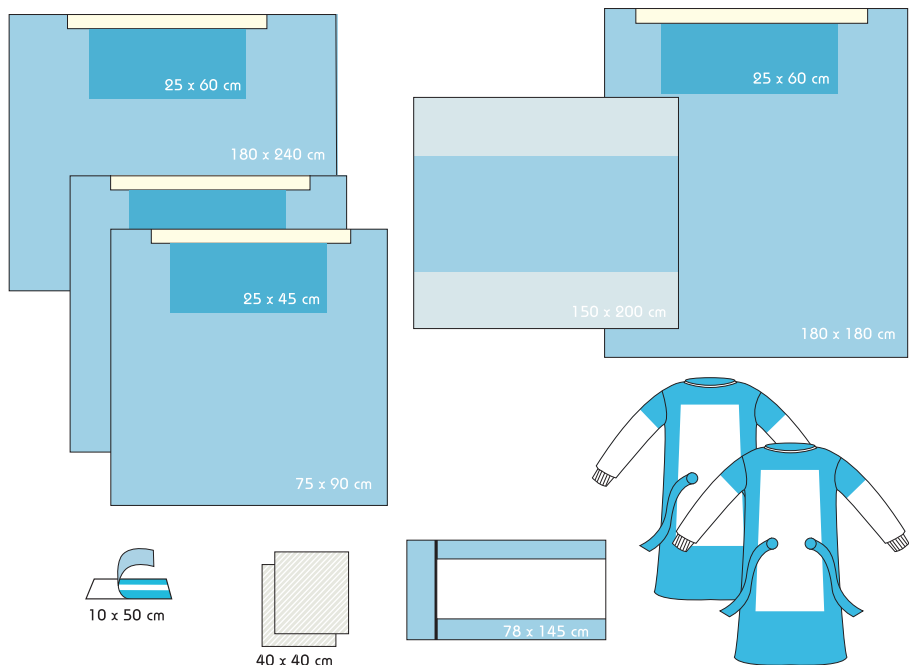

High Absorbent DL
 SMS
 Extra Absorbent
 PE Film
 Adhesive Tape





Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
ADS0011	Anesthesia Drape, Extra Absorbing 25x60 cm	180 x 240 cm	1
ADS003	Adhesive Drape, Extra Absorbing 25x45 cm	75 x 90 cm	2
ADS010	Adhesive Drape, Extra Absorbing 25x60 cm	180 x 180 cm	1
OPS001	Op-Tapes	10 x 50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RG001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

GSST003 - NG

*Product contents can be customized upon request

Laparoscopy Pack

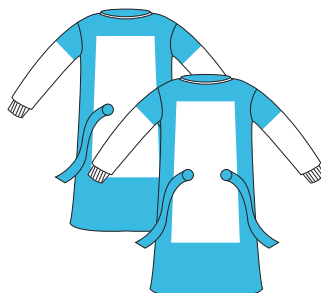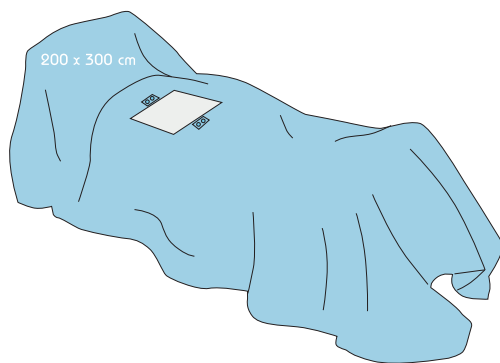

High Absorbent DL
 SMS
 PE Film
 Inscice Film
 Adhesive Tape





Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
LDS001	Laparoscopy Drape, aperture 25x30 cm	200 x 300 cm	1
OPS001	Op-Tapes	10 x 50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

LPST001 - NG

*Product contents can be customized upon request

Angiography Pack - Standard

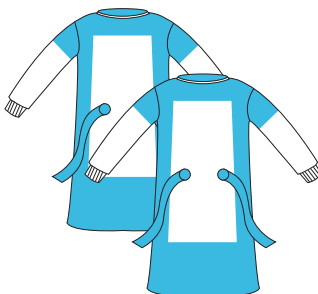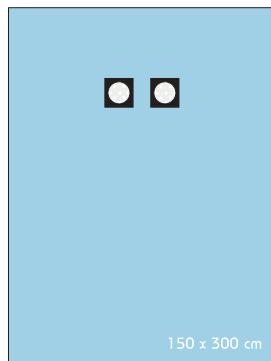

■ High Absorbent DL

■ SMS

■ PE Film

■ Inscie Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
APS002	Angiography Drape, apertures 9 cm	150 x 300 cm	1
HTS001	Hand Towels	40 x 40 cm	2
AGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

AGST001 - NG

*Product contents can be customized upon request

Angiography Pack - Large

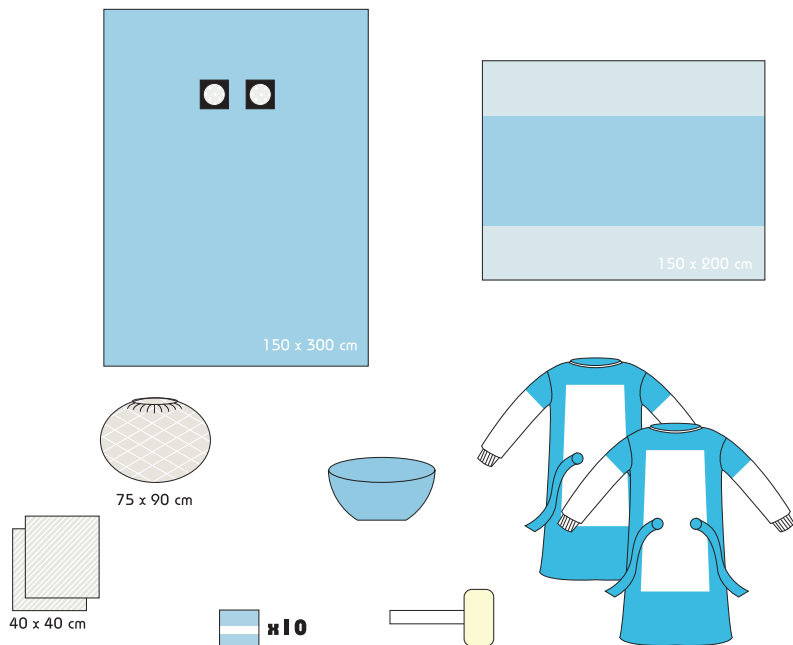

High Absorbent DL

SMS

PE Film

Insice Film





Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
APS002	Angiography Drape, apertures 9 cm	150 x 300 cm	1
FSC001	Fluoroscopy Cover, PVC	75 x 90 cm	1
BSS001	Betadine Sponge	ST	1
SCS001	Solution Cup	500 cc	1
GSS001	Gauze Swabs	7,5 x 7,5 cm	10
HTS001	Hand Towels	40 x 40 cm	2
AGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

AGST002 - NG

*Product contents can be customized upon request

Angiography Pack W / Transparent Panel Standard

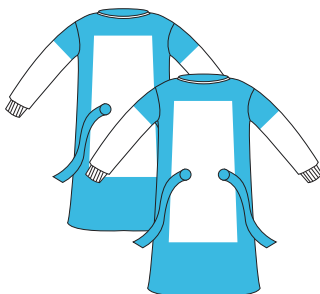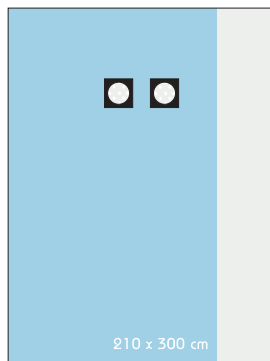

■ High Absorbent DL

■ SMS

■ PE Film

■ Inscie Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
APS001	Angiography Drape With Transparent Panel, apertures 9 cm	210 x 300 cm	1
HTS001	Hand Towels	40 x 40 cm	2
AGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

AGST003 - NG

*Product contents can be customized upon request

Angiography Pack W / Transparent Panel Large

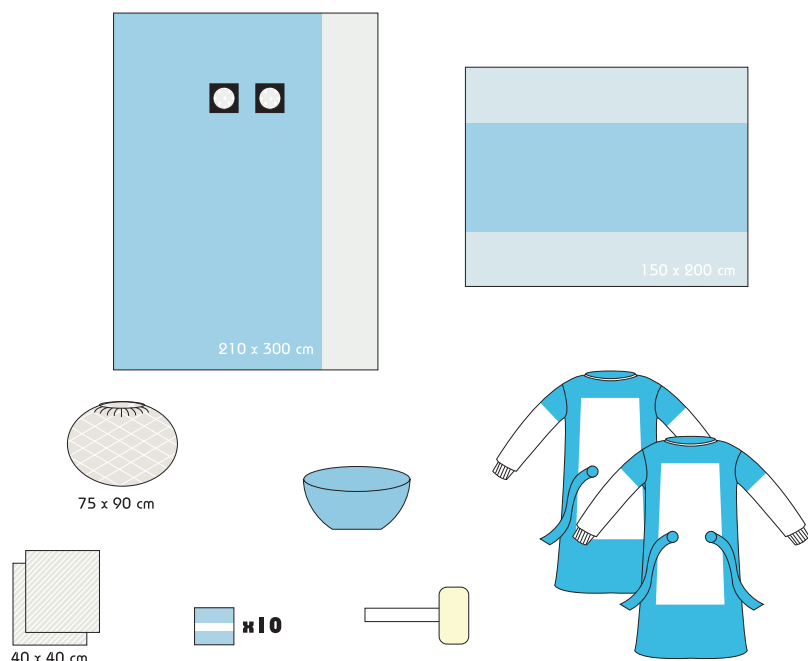

High Absorbent DL

SMS

PE Film

Inscie Film





Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
APS001	Angiography Drape With, Transparent Panel, apertures 9 cm	210 x 300 cm	1
FCS001	Fluoroscopy Cover, PVC	75 x 90 cm	1
SCS001	Solution Cup	500 cc	1
BSS001	Betadine Sponge	ST	1
GSS001	Gauze Swabs	7,5 x 7,5 cm	10
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

AGST004 - NG

*Product contents can be customized upon request

Cardiovascular Pack W / Pouch - Standard

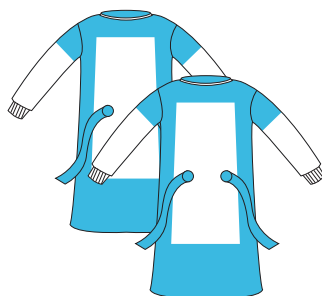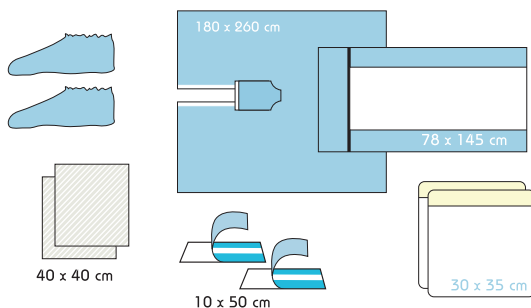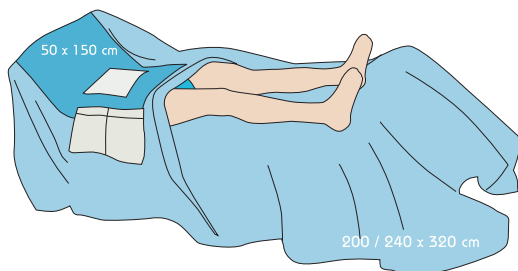

■ High Absorbent DL ■ Super Absorbent DL ■ SMS ■ PE Film ■ Insice Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
UDS003	U Split Perineal Drape, aperture 20 x 100 cm	180 x 260 cm	1
CVS002	Cardiovascular Drape, extra absorbing area 50 x 150 cm	200/240 x 320 cm	1
FSS001	Feet Socks	ST	2
OPS001	Op Tapes	10 x 50 cm	2
MPS001	Mobile PVC Bag	30 x 35 cm	2
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	Large	2

Product Code Without Gown

BPST001 - NG

*Product contents can be customized upon request

Cardiovascular Pack W / Pouch - Large

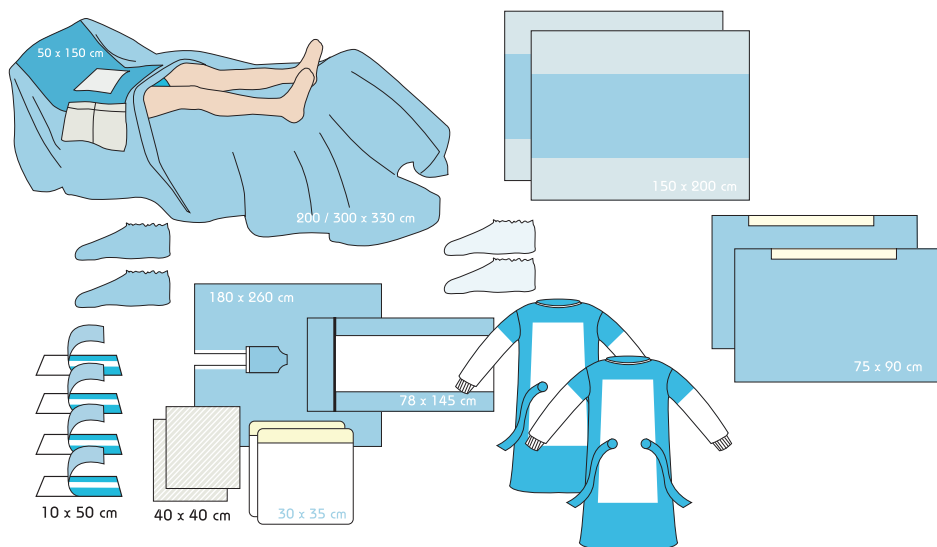

■ High Absorbent DL ■ Super Absorbent DL ■ SMS ■ PE Film ■ Inside Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	2
MYS001	Mayo Stand Cover	78 x 145 cm	1
UDS003	U Split Perineal Drape, aperture 20 x 100 cm	180 x 260 cm	1
CVS002	Cardiovascular Drape, aperture32 x 40 cm	200/300 x 330 cm	1
FSS001	Feet Socks	ST	2
FSS002	Feet Socks	Transparent	2
ADS003	Adhesive Drape	75 x 90 cm	2
OPS001	Op Tapes	10 x 50 cm	4
MPS001	Mobile PVC Bag	30 x 35 cm	2
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	Large	2

Product Code Without Gown

BPST002 - NG

*Product contents can be customized upon request

Tur Pack W / Pouch (Urology Set)

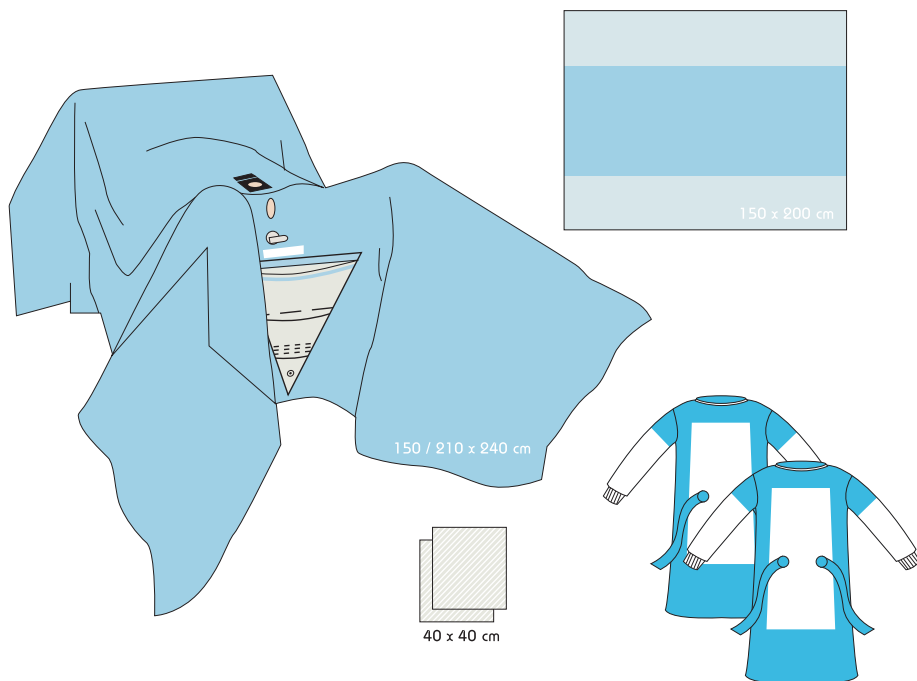

■ High Absorbent DL

■ SMS

■ PE Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
UDS001	Urology Drape W / Pouch, apertures 8 cm and 5 cm	150 / 210 x 240 cm	1
HTS001	Hand Towels	40 x 40 cm	2
AGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

TPST001 - NG

*Product contents can be customized upon request

Lithotomic Gynaecology Pack W / Pouch

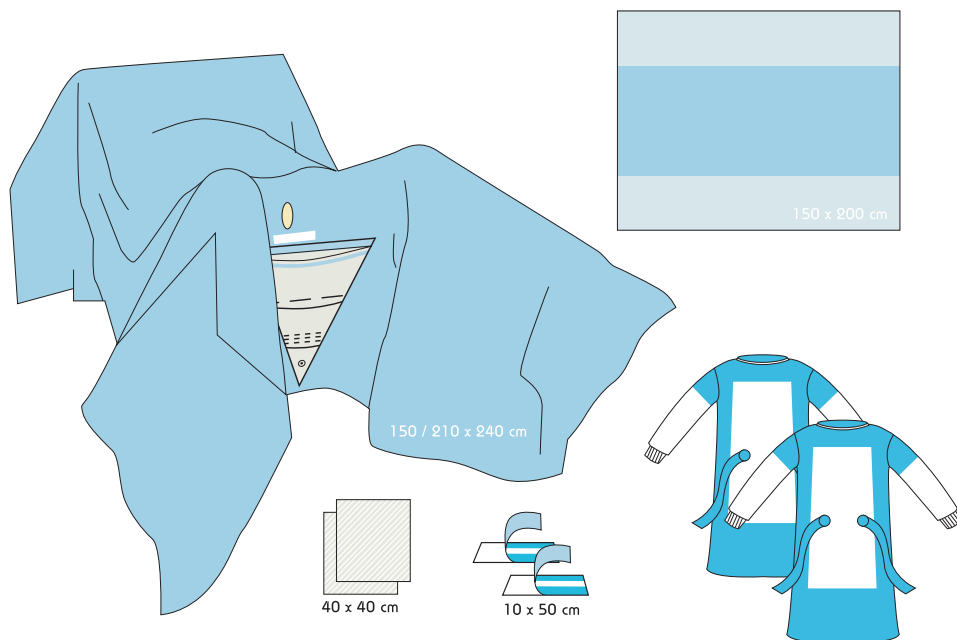

■ High Absorbent DL

■ SMS

■ PE Film





Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
UDS001	Lithotomic Gynaecology W / Pouch apertures 10 x 15 cm	150 / 210 x 240 cm	1
OPS001	Op-Tapes	10 x 50 cm	2
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

LGST001 - NG

*Product contents can be customized upon request

Gynaecology / Cystoscopy Pack

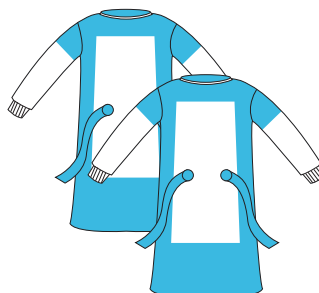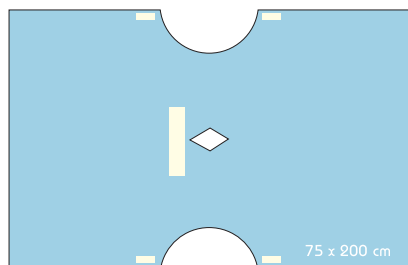

High Absorbent DL
 SMS
 PE Film
 Adhesive Tape






Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
CDS001	Cystoscopy Drape W / Adhesive Tape, apertures 10 x 15 cm	75 x 200 cm	1
LGS001	Leggings	75 x 120 cm	2
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

GCST001 - NG

*Product contents can be customized upon request

Caesarean Section Pack W / Pouch - Standard

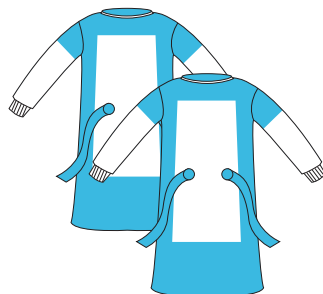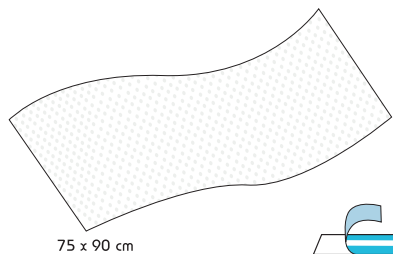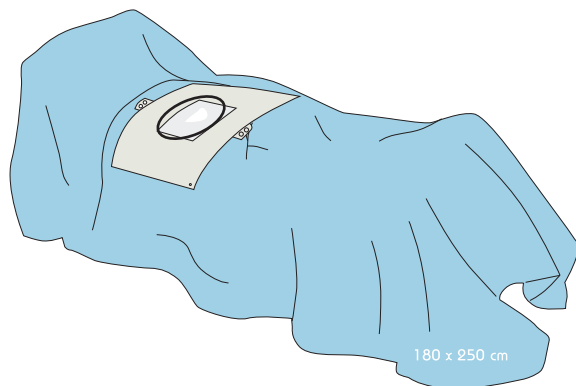

■ High Absorbent DL

■ SMS

■ PE Film

■ Insice Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
CES001	Caesarean Drape W / Pouch apertures 32 x 38 cm	180 x 250 cm	1
BBS001	Baby Blanket	75 x 90 cm	1
OPS001	Op-Tapes	10 x50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

CSST001 - NG

*Product contents can be customized upon request

Caesarean Section Pack W / Pouch - Large

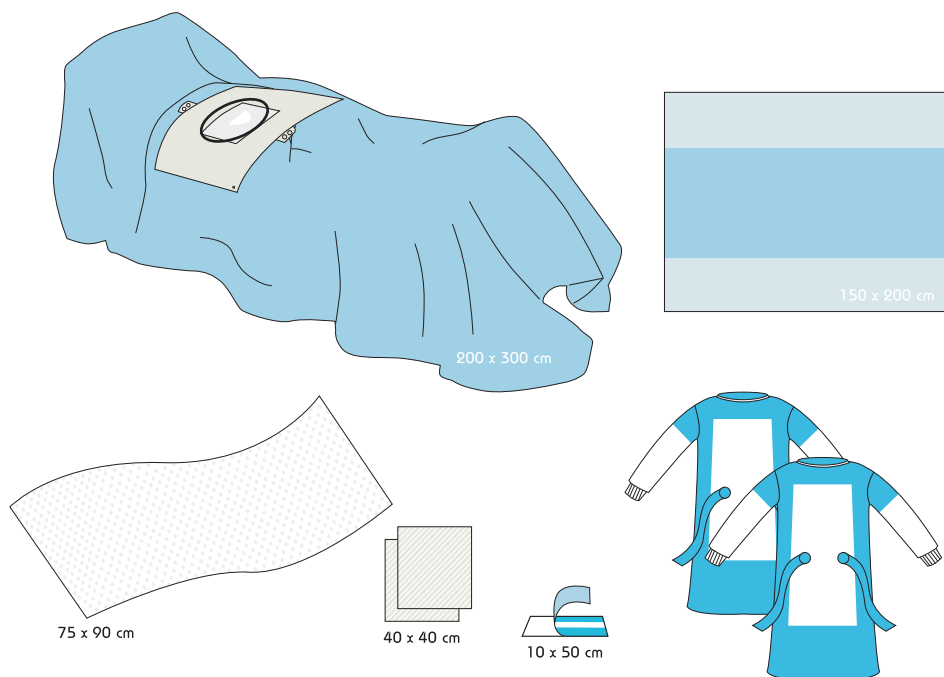

High Absorbent DL
 SMS
 PE Film
 Insice Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
CES002	Caesarean Drape W / Pouch apertures 38 x 32 cm	200 x 300 cm	1
BBS001	Baby Blanket	75 x 90 cm	1
OPS001	Op-Tapes	10 x50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

CSST002 - NG

*Product contents can be customized upon request

Caesarean Section Pack W / Pouch - Extra Large

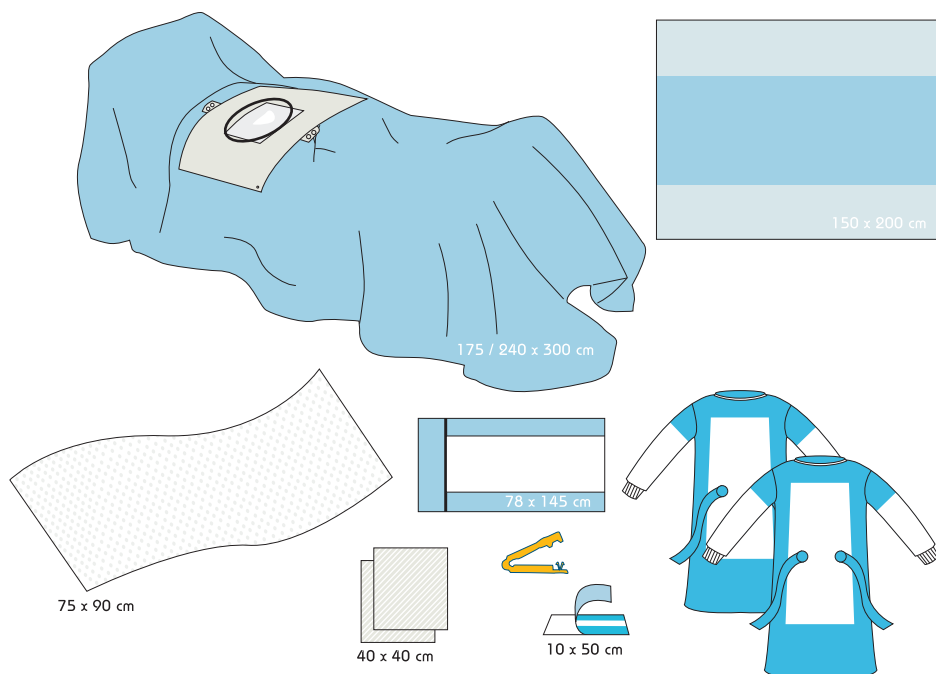

■ High Absorbent DL

■ SMS

■ PE Film

■ Inscise Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
CES003	Caesarean Drape W / Pouch apertures 38 x 32 cm	175 / 240 x 300 cm	1
BBS001	Baby Blanket	75 x 90 cm	1
CLP001	Umbilical Clamp	ST	1
OPS001	Op-Tapes	10 x50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

CSST003 - NG

*Product contents can be customized upon request

Delivery Pack

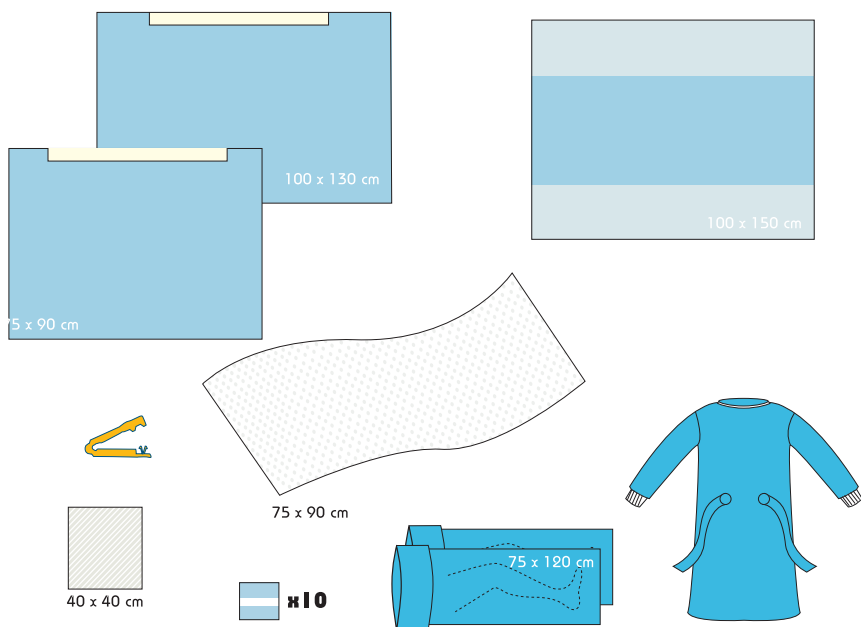

High Absorbent DL
 SMS
 PE Film
 Adhesive Tape


Codes	Description	Dimension	Quantity
ITS001	Instrument Table Cover	100 x 150 cm	1
UDS002	Underbuttock Drape	100 x 130 cm	1
ADS003	Abdominal Drape W / Adhesive Tape	75 x 90 cm	1
LGS002	Leggings	75 x 120 cm	2
CLP001	Umbilical Clamp	ST	1
BBS001	Baby Blanket	75 x 90 cm	1
GSS001	Gauze Swabs	7,5 x 7,5 cm	10
HTS001	Hand Towels	40 x 40 cm	1
SGC001	Standard Surgical Gown	LARGE	1

Product Code Without Gown

DPST001 - NG

*Product contents can be customized upon request

Delivery Pack W / Pouch

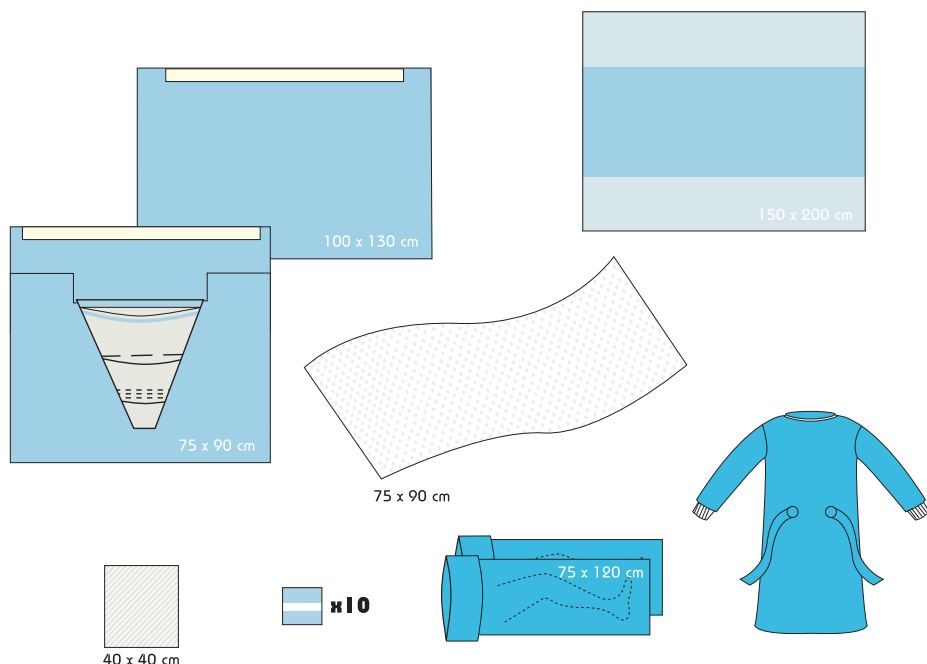

High Absorbent DL
 SMS
 PE Film
 Adhesive Tape


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
UDS001	Underbuttock Drape W / Pouch	100 x 130 cm	1
ADS003	Abdominal Drape W / Adhesive Tape	75 x 90 cm	1
LGS002	Leggings	75 x 120 cm	2
BBS001	Baby Blanket	75 x 90 cm	1
GSS001	Gauze Swabs	7,5 x 7,5 cm	10
HTS001	Hand Towels	40 x 40 cm	1
SGC001	Standard Surgical Gown	LARGE	1

Product Code Without Gown

DPST002 - NG

*Product contents can be customized upon request

Arthroscopy Pack W / Pouch - Standard

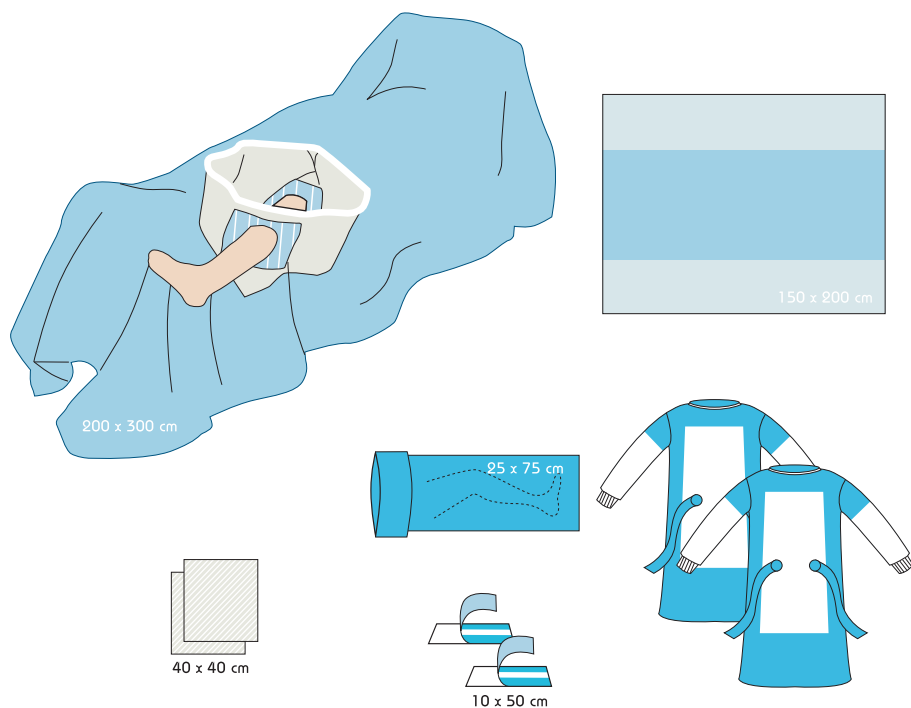

High Absorbent DL
 SMS
 PE Film
 Inscie Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
ATS001	Arthroscopy Drape W / Pouch, apertures 6 cm	200 x 300 cm	1
SSS001	Stockinet	25 x 75 cm	1
OPS001	Op-Tapes	10 x 50 cm	2
HTS001	Hand Towels	40 x 40 cm	2
RG001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

APST001 - NG

*Product contents can be customized upon request

Arthroscopy Pack W / Pouch - Large

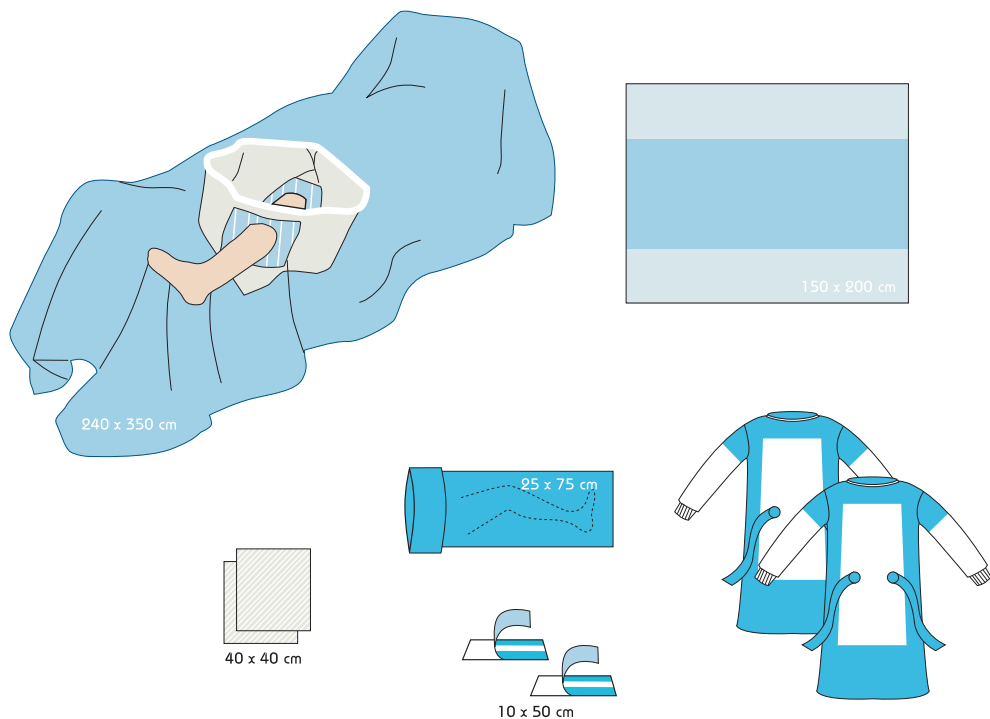

■ High Absorbent DL

■ SMS

■ PE Film

■ Insice Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
ATS001	Arthroscopy Drape W / Pouch, apertures 6 cm	240 x 350 cm	1
SSS001	Stockinet	25 x 75 cm	1
OPS001	Op-Tapes	10 x 50 cm	2
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

APST002 - NG

*Product contents can be customized upon request

Arthroscopy Pack W / Pouch - Extra Large

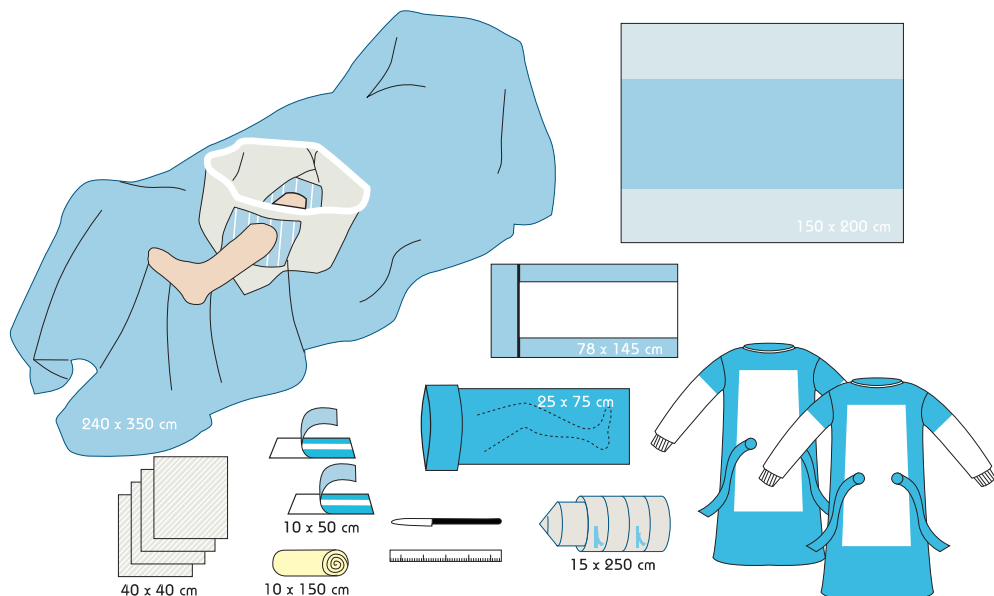

High Absorbent DL
 SMS
 PE Film
 Insice Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
ATS002	Arthroscopy Drape W / Pouch, apertures 6 cm	240 x 350 cm	1
CCS001	Camera Cover	15 x 250 cm	1
SMS001	Skin Marker and Ruler	ST	1
EBS001	Elastic Bandage	10 x 150 cm	1
SSS001	Stockinet	25 x 75 cm	1
OPS001	Op-Tapes	10 x 50 cm	2
HTS001	Hand Towels	40 x 40 cm	4
RG001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

APST003 - NG

*Product contents can be customized upon request

Craniotomy W / Pouch Pack

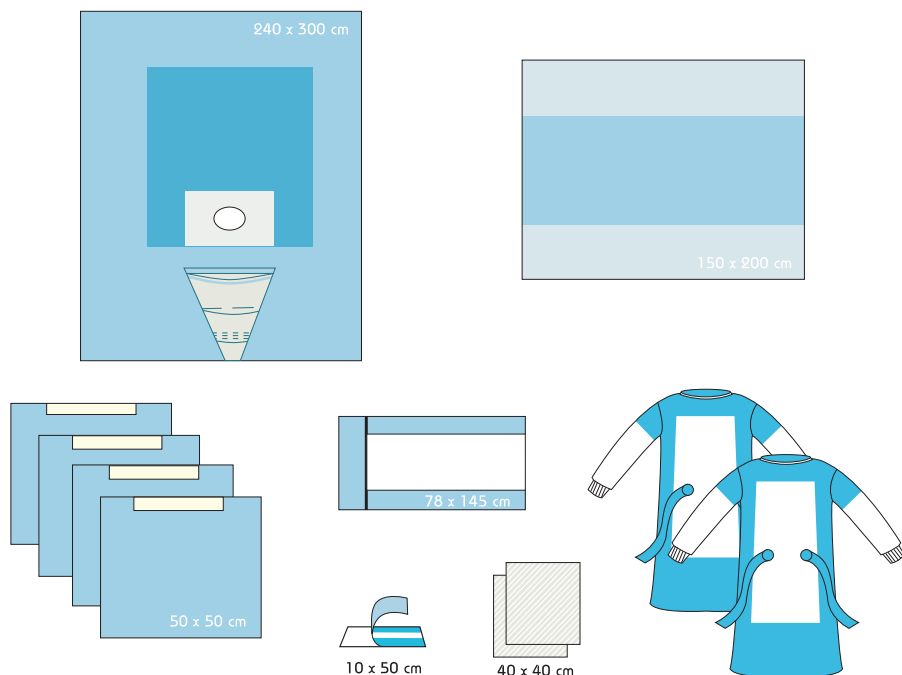

■ High Absorbent DL ■ Super Absorbent DL ■ SMS ■ PE Film ■ Adhesive Tape


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
CTS001	Craniotomy Drape W / Pouch, aperture 20 x 30 cm, extra absorbing area 75 x 90 cm	240 x 300 cm	1
ADS001	Adhesive Drape	50 x 50 cm	4
OPS001	Op-Tapes	10 x 50 cm	1
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

CANT001 - NG

*Product contents can be customized upon request

E.N.T. Pack

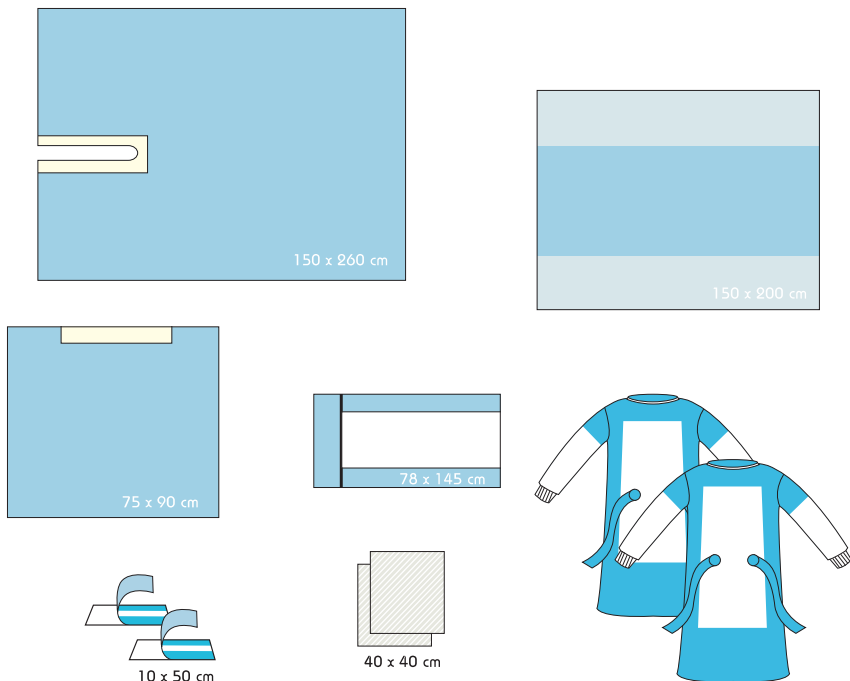

■ High Absorbent DL

■ SMS

■ PE Film

■ Inscie Film


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	1
MYS001	Mayo Stand Cover	78 x 145 cm	1
UDS001	U Split Drape, aperture 7 x 70 cm	150 x 260 cm	1
ADS003	Adhesive Drape	75 x 90 cm	1
OPS001	Op-Tapes	10 x 50 cm	2
HTS001	Hand Towels	40 x 40 cm	2
SGC001	Standard Surgical Gown	LARGE	2

Product Code Without Gown

ENST002 - NG

*Product contents can be customized upon request

Hip Pack U

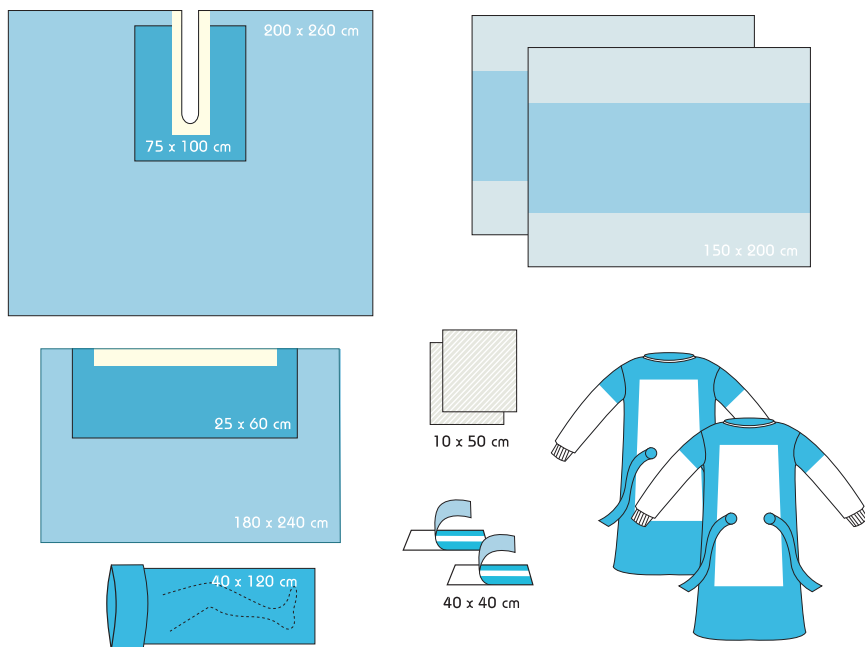

High Absorbent DL
 Super Absorbent DL
 SMS
 PE Film
 Adhesive Tape


Codes	Description	Dimension	Quantity
ITS003	Instrument Table Cover	150 x 200 cm	2
UDS001	U Split Drape, aperture 20 x 100 cm, extra absorbing area 75 x 100 cm	200 x 260 cm	1
ADS011	Adhesive Drape, extra absorbing area 25 x 60 cm	180 X 240 cm	1
LGS003	Leggings	40 x 120 cm	1
OPS001	Op-Tapes	10 x 50 cm	2
HTS001	Hand Towels	40 x 40 cm	2
RGC001	Reinforced Surgical Gown	LARGE	2

Product Code Without Gown

HUST001 - NG

*Product contents can be customized upon request

Implant Pack

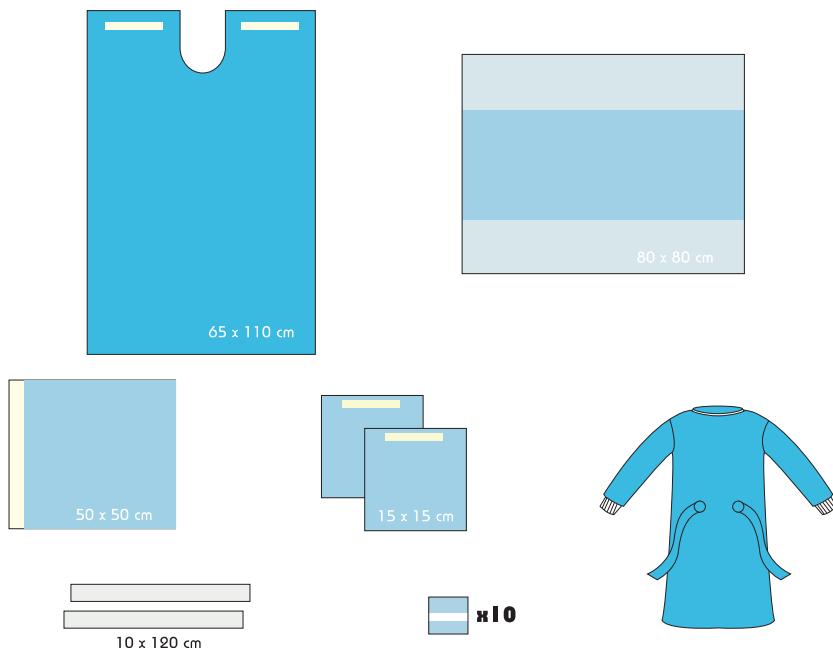

■ High Absorbent DL ■ SMS ■ PE Film ■ Adhesive Tape





Codes	Description	Dimension	Quantity
ITS002	Instrument Table Cover	80 x 80 cm	1
DPS001	Dental Patient Gown W / Velcro	65 x 110 cm	1
TDS001	Table Drape	50 x 50 cm	1
RDS001	Reflector Drape	15 x 15 cm	2
THS001	Transparent Hose Cover	10 x 120 cm	2
GSS001	Gauze Swabs	7,5 x 7,5 cm	10
SGC001	Standard Surgical Gown	LARGE	1

Product Code Without Gown

IPST001 - NG

*Product contents can be customized upon request

Single Pouch Ophthalmic Pack

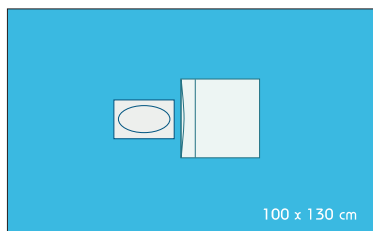

■ SMS

■ PE Film

■ Inside Film

Codes	Description	Dimension	Quantity
ITS001	Instrument Table Cover	100 x 150 cm	1
ODS001	Single Pouch Ophthalmic Drape W / Pouch, aperture 10 x 10	100 x 130 cm	1
HTS001	Hand Towels	40 x 40 cm	2
SGC001	Standard Surgical Gown	LARGE	1

Product Code Without Gown

OPST001 - NG

*Product contents can be customized upon request


Adhesive Drapes



■ High Absorbent DL ■ Adhesive Tape

Codes	Description	Dimension
ADS001	Adhesive Drape	50 x 50 cm
ADS002	Adhesive Drape	75 x 75 cm
ADS003	Adhesive Drape	75 x 90 cm
ADS004	Adhesive Drape	75 x 150 cm
ADS005	Adhesive Drape	100 x 100 cm
ADS006	Adhesive Drape	120 x 150 cm
ADS007	Adhesive Drape	120 x 240 cm
ADS008	Adhesive Drape	150 x 180 cm
ADS009	Adhesive Drape	150 x 240 cm
ADS010	Adhesive Drape	180 x 180 cm
ADS011	Adhesive Drape	180 x 240 cm

Non Sterile Welcome Pack (Waterproof)

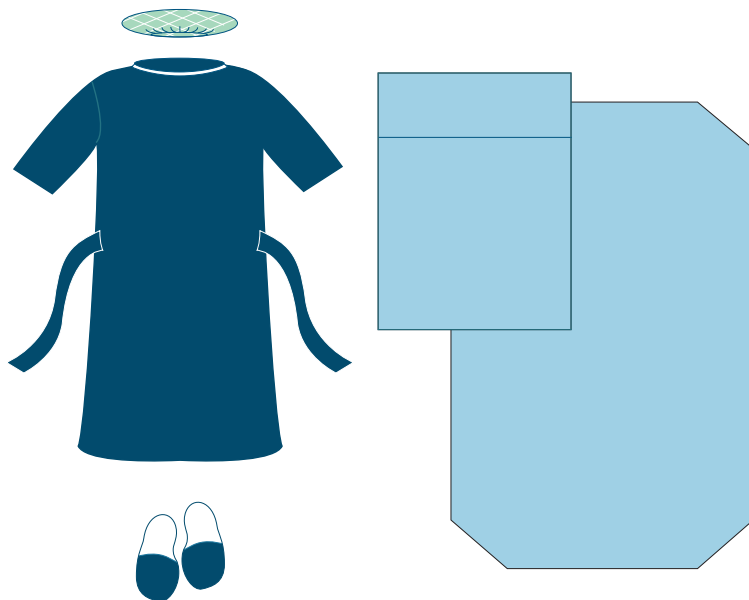

■ PP

■ SMS

Codes	Description	Dimension	Quantity
BCNS001	Bed Cover W / Elastic Edges	160 x 240 cm	1
PCNS001	Pillow Cover	50 x 70 cm	1
SLPNS	Slippers	ST	1
PGNSS001	Patient Gown Short Sleeve	LARGE	1
SBCNS001	Soft Bar Caps	ST	1

Product Code Without Gown

WPNS001 - NG

*Product contents can be customized upon request

Broche[®]

Procedure Packs



Description	Quantity
Paper or SMS wrap	1
Back table cover to wrap	1
Back table cover book folded	1
Mayo stand cover	1
Instrument diathermy pouch	1
Kidney bowl 700ml	1
Blade 21	1
Blade 23	1
Bowl 500ml	1
Bowl 1000ml	1
Bowl 250ml	2
Jug 1000ml	1
Cautery pencil	1
Cautery quiver	1
Cautery tip cleaner	1
Light handle cover	2
Incise or ioban	1
Drape laparotomy	1
Skin marker	1
Suction Yankauer	1
Suction tubing	2
Needle counter box or pad	2
Swab gauze small X-ray tied 5's	2
Swab gauze large X-ray tied 5's	2
Hand towel	1
Drape medium plain	2
Op tape	2
Dressing pad	1
Dressings adhesive	1

Description	Quantity
Namic™ 2 port manifold	1
Galipot 120ml	2
Guidewire bowl	1
Syringe, P.É, 10ml, US	4
Syringe, P.É, 5ml, US	1
Label set	1
Needle 18G x 7cm (70mm) introducer needle	1
Needle 21G x 3.8cm hypo green	1
Needle 23G x 3cm hypo blue	1
Scalpel No.11	1
Sponge stick medium 15cm	2
Swab gauze, 10 x 10cm, 12ply, 10 pack	1
Medium fluoro cover	1
Sharps needle containment device	1
Angio drape, 2 fenestrations, 3 ply laminate, no windows, 300cm	1
Equipment cover, P.É, 100 x 100cm	1
Bowl 250ml	1
Sponge bowl 500ml	1

Description	Quantity
Paper or SMS wrap	1
Back table cover to wrap	1
Back table cover book folded	1
Bowl 6000ml or bowl liner	1
Baby blanket	1
Blade 21	1
Blade 23	1
Bowl 500ml	1
Umbilical clamp	1
Mayo stand cover	1
Cautery diathermy pencil	1
Drape medium plain	1
Drape C section	1
Light handle cover	2
Suction Yankauer	1
Needle counter box or pad	1
Maternity pad	1
Swab gauze small X-ray (5's)	1
Swab gauze large X-ray (5's)	2
Syringe 60ml catheter tip	1
Suction tubing	2
Adhesive dressing	1
Dressing pad	1
Placenta bowl	1

Description	Quantity
Paper or SMS wrap	1
1 Back table cover to wrap	1
2 Back table cover book folded	2
1 Mayo stand cover	1
1 Instrument diathermy pouch	1
2 Kidney bowl 700ml	2
1 Blade 20	1
1 Blade 21	1
2 Blade 23	2
1 Bowl 500ml	1
1 Bowl 1000ml	1
2 Bowl 250ml	2
1 Jug 1000ml	1
1 Cautery diathermy pencil	1
1 Cautery diathermy quiver	1
1 Cautery diathermy tip cleaner	1
1 Cautery diathermy blade	1
3 Dressings adhesive	3
2 Bandage crepe 15cm	2
2 Bandage crepe 10cm	2
5 Vessel loops various colours	5
10 Suture boots	10
2 Light handle cover	2
1 Incise or ioban	1
1 Drape cardiovascular	1
1 Drape double split	1
1 Drape foot covers pair	1
1 Drape head / large with adhesive edge	1
2 Drape medium plain	2
4 Drape small plain utility	4
1 Dressings adhesive	1
1 Skin marker	1
2 Suction Yankauer	2
1 Handle suction frazier	1
1 Suction tubing	1
1 Needle counter box or pad	1
2 Swab gauze small X-ray tied 5's	2
2 Swab gauze large X-ray tied 5's	2
1 Skin staples 35 wide	1
2 Hand towel	2
2 Steri strips wide	2
2 Op tape	2
1 Dressing pad	1
2 Huck towels blue	2

Description	Quantity
Paper or SMS wrap	1
Back table cover to wrap	1
Kidney bowl 800ml	1
Blade 11	1
Blade 15	1
Drape legging	2
Bowl 1000ml	1
Mayo stand cover	1
Gallipot 120ml	1
Under buttock drape	1
Insufflation tubing	1
Veress needle	1
Fog free solution	1
Light handle cover	2
Suction Yankauer	1
Suction tubing	1
Needle counter box or pad	1
Maternity pad	1
Swab gauze small X-ray tied 5's	2
Hand towel	1
Velcro strip	1
Adhesive dressing	2
Drape w/ adhesive edge	1
Camera cover	1

Description	Quantity
Paper or SMS wrap	1
1 Back table cover to wrap	1
1 Bowl 1000ml	1
1 Gallipot 120ml	1
1 Kidney bowl 800ml	1
1 Jug 1000ml	1
1 Drape TUR	1
1 Irrigation tubing set	1
2 Swab gauze small X-ray tied 5's	2
2 Velcro strip	2
1 Camera cover	1
1 Suction tubing	1
2 Hand towels	2
1 Ellik bladder evacuator	1

Description	Quantity
Paper or SMS wrap	1
1 Back table cover to wrap	1
1 Back table cover book folded	1
1 Mayo stand cover	1
2 Kidney bowl 800ml	2
2 Blade 23	2
1 Blade 20	1
1 Bandage crepe 15cm	1
1 Bowl 500ml	1
1 Bowl 1000ml	1
1 Cautery pencil	1
1 Cautery tip cleaner	1
1 Cautery quiver	1
2 Bowl 250ml	2
1 Drape elliptical hip	1
1 U drape	1
1 Ioban	1
2 Light handle cover	2
1 Suction Yankauer	1
1 Suction tubing	1
1 Skin marker C/W ruler	1
1 Needle counter box or pad	1
1 Jug 1000ml	1
1 Instrument diathermy pouch	1
5 Swab gauze small X-ray tied 5's	5
10 Swab gauze large X-ray tied 5's	10
1 Stockinette (cotton/impervious)	1
1 Syringe 60ml catheter tip	1
1 Dressing adhesive	1
1 Dressing pad	1
1 Op tape	1
1 Drape medium plain	1

Description	Quantity
Paper or SMS wrap	1
Back table cover to wrap	1
Kidney bowl 800ml	1
Blade 11	1
Bandage crepe 15cm	1
Bowl 500ml	1
Bowl 250ml	2
Drape arthroscopy	1
Stockinette (cotton/impervious)	1
Skin marker	1
Needle counter box or pad	1
Needle white ivory 19g 5cm	1
Bandage ortho padding 15cm	1
Swab gauze small X-ray tied 5's	5
Syringe 20ml LS	1
Suction tubing	1
Op tape	1
Drape medium plain	1
Camera cover	1

Description	Quantity
Back table cover to wrap	1
1 Mayo stand cover	1
1 Kidney bowl 700ml	1
1 Bowl 500ml	1
1 Gallipot 60ml	1
1 Drape ophthalmic	1
1 Eye spears (10 pack)	1
1 Needle counter box or pad	1
1 Needle orange 25G 5/8 inch	1
1 Needle yellow 30G 1/2 inch	1
1 Eye pad	1
1 Eye shield clear	1
2 Swab gauze small X-ray tied 5's	2
1 Syringe 1ml LS	1
1 Syringe 5ml LL	1


Broche[®] Gowns





STERILE GOWNS

Disposable Sterile Ultrasonic Stitch Surgical Gown

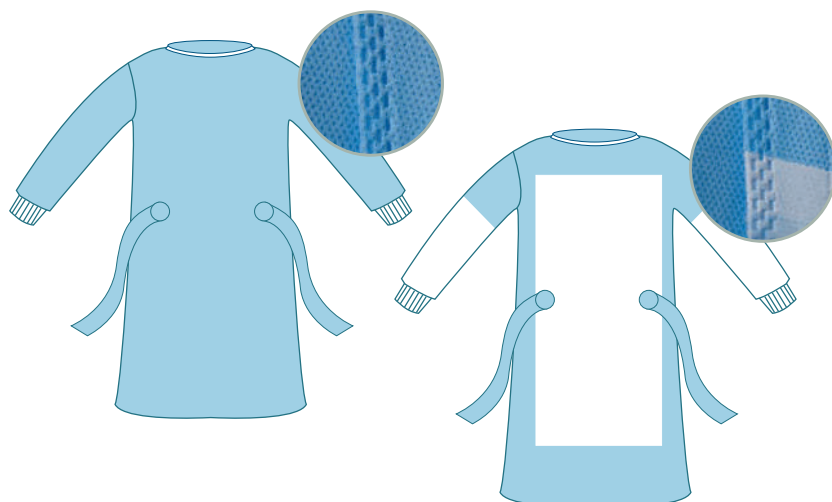

COLOR



BLUE

DESCRIPTION	SIZE	CODE
SMS/SSMMS STERILE ULTRASONIC STITCH STANDARD SURGICAL GOWN W/A TOWEL	L - XL	SGC001 - SGC002
SMS/SSMMS STERILE ULTRASONIC STITCH REINFORCED SURGICAL GOWN W/A TOWEL	L - XL	RGC001 - RGC002

GOWNS DETAILS

The surgical gowns are sterilized with ethylenoxide and are designed to cover the surgeon during surgical operations. The gowns are classified into two types according to the duration of the surgical operations and also according to the type of selected material - SMS/SSMMS - and each of them may be equipped with liquid resistant lining. The elastic cuff on the sleeves are made from 95% cotton, 5% spandex.

- Water resistant
- Easy fit
- Comfortable design
- Air permeable
- Ultrasonic stitch

Gowns have the quality to allow respiration, and retain and repel alcohol, blood, water and any kind of body fluids without absorbing them. Gowns, which are produced with no-shred and non-woven SMS/SSMMS fabric, do not let soaking up, thus, prevents infection spread, and provide a healthy and comfortable work environment for medical personnel.



NON-STERILE GOWNS

Disposable Non-Sterile Patient Gown



COLOR




NAVY



BLUE

DESCRIPTION	SIZE	CODE
NON-STERILE PATIENT GOWN (LONG SLEEVE)	L - XL	PGL001 - PGL002
NON-STERILE PATIENT GOWN (SHORT SLEEVE)	L - XL	PGS001 - PGS002

Disposable Non-Sterile Doctor Scrub Suits

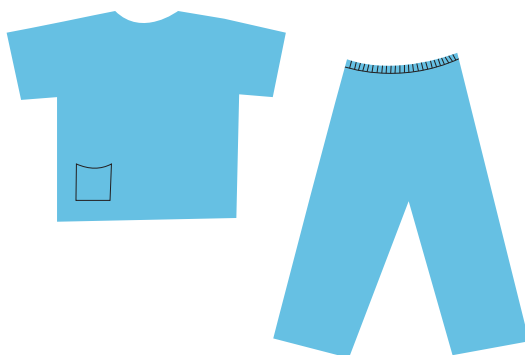

COLOR



BLUE

DESCRIPTION	SIZE	CODE
NON-STERILE DISPOSABLE DOCTOR SCRUB SUITS	L - XL	DSS001 - DSS002

Broche[®] *Gloves*



STERILE GLOVES

Chloroprene Synthetic Sterile Surgical Gloves **NEO+PLUS**



DESCRIPTION

POWDER FREE
LATEX FREE, NON-ALLERGIC
BEADED CUFF
FOR SINGLE USE ONLY
50 PAIRS PER BOX
AQL 1.5
STERILE **R**

SIZE

6,5 - 7 - 7,5 - 8 - 8,5

COLOR



BROWN

STERILE GLOVES

Latex Sterile Surgical Gloves **+PLUS**



DESCRIPTION

POWDERED and POWDER FREE
BEADED CUFF
TEXTURED
WEIGHT REFERENCE SIZE 7,5: 16,8 gr/pair
FOR SINGLE USE ONLY
50 PAIRS PER BOX
AQL 1,5
STERILE **R**

SIZE

6,5 - 7 - 7,5 - 8 - 8,5

COLOR



NATURAL

NON-STERILE GLOVES

Latex Examination Gloves



DESCRIPTION

POWDERED
SMOOTH SURFACE
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX

SIZE

XS - S - M - L

COLOR



NATURAL



NON-STERILE GLOVES

Latex Examination Gloves



DESCRIPTION

POWDER FREE
TEXTURED
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX

SIZE

S - M - L

COLOR



NATURAL



NON-STERILE GLOVES

Vinyl Examination Gloves



DESCRIPTION

POWDERED
LATEX FREE
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX
AQL 1,5

SIZE

S - M - L

COLOR



CLEAR

NON-STERILE GLOVES

Vinyl Examination Gloves



DESCRIPTION

POWDER FREE
LATEX FREE
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX
AQL 1,5

SIZE

S - M - L

COLOR



CLEAR



LATEX LIKE



BLUE



NON-STERILE GLOVES

Nitrile Examination Gloves



DESCRIPTION

POWDER FREE
LATEX FREE, NON ALLERGIC
FINGER TEXTURED
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX
AQL 1,5

SIZE

S - M - L

COLOR



NON-STERILE GLOVES

Nitrile Chemotherapy Examination Gloves



DESCRIPTION

POWDER FREE
LATEX FREE, NON ALLERGIC
TESTED FOR USE WITH CHEMOTHERAPY DRUGS
4 MIL - 12" CUFF
FINGER TEXTURED
BEADED CUFF
AMBIDEXTROUS
FOR SINGLE USE ONLY
100 PCS PER BOX
AQL 1,5

SIZE

S - M - L

COLOR



BLUE



NON-STERILE GLOVES

PE Gloves



DESCRIPTION

FOR SINGLE USE ONLY
WEIGHT 7 KG / 10.000 pcs
100 PCS PER BAG

SIZE

L

COLOR



CLEAR

Broche[®] Plastic Products



PLASTIC PRODUCTS

Sterile Flowmeter



DESCRIPTION	DESCRIPTION
MATERIAL: MEDICAL GRADE POLY VINYL CHLORIDE	LUER LOCK
DROPPING VARIATION 5 TO 250 ML/h	FOR SINGLE USE ONLY
LATEX FREE	INDIVIDUAL PACKING
Y INJECTION PORT	EO STERILE

Sterile Infusion (Serum) Set



DESCRIPTION	DESCRIPTION
MATERIAL: MEDICAL GRADE POLY VINYL CHLORIDE	WITH AIR VENT
WITH DRIP CHAMBER	FOR SINGLE USE ONLY
APPOPRIATE FOR INFUSION BOTTLES AND ALSO FOR INFUSION BAGS	INDIVIDUALLY PACKED IN PE BAG
FILTER IN DRIP CHAMBER	EO STERILE
WITH A FLOW REGULATOR	

PLASTIC PRODUCTS

Sterile Urine Bag / T-Valve and Push & Pull Valve



DESCRIPTION

MATERIAL: MEDICAL GRADE PVC

2000 ML COLLECTING CAPACITY

WITH ANTI-REFLUX VALVE

REINFORCED HOLES FOR HANGING

LATEX FREE

FOR SINGLE USE ONLY

INDIVIDUALLY PACKED IN PE BAG

EO STERILE

PLASTIC PRODUCTS

Sterile Blood Transfusion Set



DESCRIPTION

MATERIAL: MEDICAL GRADE POLY VINYL CHLORIDE

WITH FLOW REGULATOR

WITH BLOOD FILTER

NON TOXIC and NON PYROGENIC

18 G HYPODERMIC NEEDLE

WITH AIR VENT

FOR SINGLE USE ONLY

INDIVIDUALLY PACKED IN PE BAG

EO STERILE

Broche[®] *Medical Disposables*



MEDICAL DISPOSABLES

Sterile Surgical Blades



DESCRIPTION

MATERIAL: CARBON STEEL

NO: 10 - 11 - 12 - 15 - 18 - 20 - 21 - 22 - 23 - 24 - 25

FOR SINGLE USE ONLY

100 PCS PER BOX

STERILE **R**



MEDICAL DISPOSABLES

Sterile Blood Lancet



DESCRIPTION

MATERIAL: CARBON STEEL

DISPOSABLE

FOR SINGLE USE ONLY

200 Pcs PER BOX

STERILE **A**



MEDICAL DISPOSABLES

Sterile / Non-Sterile Wooden Tongue Depressor



DESCRIPTION	SIZE
MATERIAL: BIRCH TREE	ADULT 150mm X 18mm
SMOOTH SURFACE WITH ROUND ENDS	
FOR SINGLE USE ONLY	
100 PCS PER BOX	

MEDICAL DISPOSABLES

Shoe Covers



DESCRIPTION

MATERIAL: POLYETHYLENE
FOR SINGLE USE ONLY
100 PCS PER PACKET

COLOR



BLUE



MEDICAL DISPOSABLES

Face Mask



DESCRIPTION

MATERIAL: NONWOVEN POLYPROPYLENE SPUNBONDED FABRIC

2 PLY AND 3 PLY

ULTRASONIC STITCH

WITH ROUND ELASTIC EARLOOP OR WITH POLYPROPYLENE TIE

NOSE SUPPORT

FOR SINGLE USE ONLY

50 PCS PER BOX

COLOR



GREEN



WHITE



MEDICAL DISPOSABLES

Soft Bar Cap



DESCRIPTION

MATERIAL: NONWOVEN POLYPROPYLENE SPUNBONDED FABRIC
ULTRASONIC STITCH
DOUBLE ELASTIC
FOR SINGLE USE ONLY
100 PCS PE BAG

SIZE

21 INCH

COLOR



GREEN



WHITE

EC CERTIFICATE

AT SERTİFİKA

According to Annex II of the Directive 93/42/EEC on Medical Devices

93/42/AT Tıbbi Cihaz Yönetmeliği Ek II'ye göre

Full Quality Assurance System

Tam Kalite Güvence Sistemi

Certificate Number: 2195-MED-1412002

Sertifika Numarası

Manufacturer:

Üretici

NURTEKS TEKSTİL NAKİŞ SAN. VE TİC. LTD. ŞTİ.

Koşklü Çeşme Mah. Yeni Bağdat Cad. No:124 Gebze Kocaeli TURKEY

Product(s):

Ürün(ler)

Sterile Disposable Surgical Drape, Gown and Drape Sets

Steril Tek Kullanımlık Cerrahi Örtü, Önlük ve Örtü Setleri

Sterile Disposable Powder and Powder-Free Surgical Latex Gloves

Steril Tek Kullanımlık Pudralı ve Pudrasız Cerrahi Lateks Eldivenler

Final Report No:

Final Raporu Numarası

2195-MED-1404008 , 2195-MED-1502010

Szuteş, Notified Body 2195, declares that the aforementioned manufacturer has implemented a quality assurance system according to Annex II, Section 3 (excluding section 4) of the directive 93/42/EEC on medical devices. This quality assurance system covers those aspects of manufacturing concerned with securing and maintaining safe conditions of the respective product(s) and conforms to the provisions of this Directive. The approved quality system is subject to surveillance pursuant to Annex II Section 5 of Directive 93/42/EEC.

Szuteş must be informed of any significant changes in the design and/or construction of the product(s).

2195 kimlik numaralı Onaylanmış Kuruluş Szuteş, yukarıda belirtilen üreticinin 93/42/AT Tıbbi Cihaz Yönetmeliği EK II madde 3 (madde 4 hariç) 'üne göre bir kalite yönetim sistemi uyguladığını, bu yönetim sisteminin yönetmeliğin sadece bahsi geçen ürünlerin üretiminin güvenlik koşullarını sağlama ve devam ettirme ile ilgili gerekliliklerini karşıladığını beyan eder. Onaylanan bu kalite yönetim sistemi, 93/42/AT Tıbbi Cihaz Yönetmeliği EK II, Madde 5'e göre periyodik olarak gözetime tabidir.

Üretici, ürünlerinin tasarımı ve yapısında gerçekleştirdiği önemli değişiklikleri Szuteş'e bildirmek zorundadır.

This EC certificate is valid till 2019.04.29

Bu AT Sertifikası 2019.04.29 tarihine kadar geçerlidir

Istanbul, 2014.04.30

Rev.01, 2015.02.27



Özgür Vıdan
Deputy General Manager
Genel Müdür Yardımcısı





TÜRK STANDARDLARI ENSTİTÜSÜ
TÜRK STANDARDLARINA UYGUNLUK BELGESİ
TURKISH STANDARDS INSTITUTION
CERTIFICATE OF CONFORMITY TO TURKISH STANDARDS

Markanın Tanımı Description of the Mark
TSE veya/or  veya/or T S E

BELGE NUMARASI
REFERENCE NUMBER OF LICENCE

14.0.30.4.34.00/TSE-65761

BELGENİN İLK VERİLİŞ TARİHİ
DATE OF FIRST ISSUE OF LICENCE

15.04.2014

BELGENİN SON GEÇERLİLİK TARİHİ
LICENCE VALID UNTIL

15.04.2016

BELGE SAHİBİ KURULUŞUN ADI
NAME OF THE LICENCE HOLDER

NURTEKS TEKSTİL NAKİŞ SANAYİ VE TİCARET LIMITED ŞİRKETİ

BELGE SAHİBİ KURULUŞUN ADRESİ
ADDRESS OF THE LICENCE HOLDER

TURGUT REİS MAH. TEKSTİLKENT KOZA PLAZA İŞ MERKEZİ
B-BLOK KAT.3 NO:11 ESENLER İSTANBUL/TÜRKİYE

ÜRETİM YERİ ADI
NAME OF THE MANUFACTURING PLACE

NURTEKS TEKSTİL NAKİŞ SAN. TİC. LTD. ŞTİ.

ÜRETİM YERİ ADRESİ
ADDRESS OF THE MANUFACTURING PLACE

KÖŞKLÜÇEŞME MAHALLESİ
YENİ BAĞDAT CADDESİ
NO : 124 GEBZE / KOCAELİ
KOCAELİ/TÜRKİYE

İPTAL EDİLEN BELGE NUMARASI (Varsa)
INDICATION OF SUPERSEDED LICENCE (if any)

TESCİLLİ TİCARİ MARKASI
REGISTERED TRADE MARK

BROCHE

İLGİLİ TÜRK STANDARDI
RELATED TURKISH STANDARD

TS EN 13795+A1 / Surgical drapes, gowns and clean air suits, used as medical devices for patients, clinical staff and equipment - General requirements for manufacturers, processors and products, test methods, performance requirements and performance levels / 12.06.2013

BELGE KAPSAMI
SCOPE OF LICENCE

SURGICAL DRAPES, GOWNS AND CLEAN AIR SUITS, USED AS MEDICAL DEVICES, FOR PATIENTS, CLINICAL STAFF AND EQUIPMENT - PART1: GENERAL REQUIREMENTS FOR MANUFACTURERS, PROCESSORS AND PRODUCTS

SURGICAL DRAPES
-SINGLE-USE PRODUCT (TABLE 2)
-HIGH PERFORMANCE
-CRITICAL PRODUCT AREA



13/05.2015


HAKAN DENİZ
MANAGER OF THE İSTANBUL
CERTIFICATION DEPT.

*Bu belge, Belgelendirilen Ürünün, Üretimin Yürütülmesi Enstitümüzün belirlenmiş şartları karşıladığını da gösterir.

*Bu belge hiç bir şekilde tıbbi amaçlarla, insanlara veya okyanuslara zarar vermesi için kullanılmamalıdır, ayrıca ne satılmalı yapılmamalıdır.

*İSTANBUL - İSTANBUL BELGELENDİRME MÜDÜRLÜĞÜ * Çayyolu Tirm Binası Yarı Çayyolu/GEZİTİ * Tel: 3527231273 * Faks: 3527231006 * Web: * e-mail:

*ANKARA - BELGELENDİRME MERKEZİ BAĞKURULUĞU Necatibey Cad. No:112 06100 Beşikdüzü/ANKARA - web: www.tse.org.tr



SERTİFİKA / CERTIFICATE

NURTEKS TEKSTİL NAKİŞ SAN. VE TİC. LTD. ŞTİ.

Address: Köşklü Çeşme Mah.Yeni Bağdat Cad. No:124 Gebze Kocaeli Türkiye
Scope:

Production of Disposable; Sterile Surgical Gowns and Drapes, Nonsterile Gowns and Drapes

Sale of Disposable Sterile Products; (Surgical Gloves, Wooden Tongue Depressor, Surgical Blades, Flowmeter, Infusion (Serum) Set, Urine Bag, Blood Transfusion Set, Blood Lancet)

Sale of Disposable Nonsterile Products; (Examination Gloves, PE Gloves, Mask, Caps, Shoe Covers, Wooden Tongue Depressor, Underpads, Gowns and Drapes, Non-Woven PP Fabrics)

Clauses are excluded: 7.3

Certificate No: NİS 991-02

Issuing Place and Date: ANKARA-06.05.2014

EN ISO 9001:2008

Quality Management System

Nissert has verified that the organisation above has established and applies a Quality Management System. If certification conditions of NİSSERT, and requirements of this Standard are obeyed and surveillance audits are carried out; this certificate is valid until **05.05.2017**

1. Surveillance Audit Visa: 19.04.2015

2. Surveillance Audit Visa: 19.04.2016

[Signature]
On Behalf of Nissert

You can observe the information of the validation of this certificate from the phone or e-mail address which are below. When surveillance audits are done, stamp is taped on relevant space and signed. Certificates which aren't stamped and signed after the date of surveillance audit are invalid.



Adres: Gimat 3. Blok No 29 PK 06370
Mecanköy Ankara - Türkiye
Tel: 0312-397 00 09-397 07 87
Fax: 0312-397 00 58 E-mail: nissert@nissert.com





SERTİFİKA / CERTIFICATE

NURTEKS TEKSTİL NAKİŞ SAN. VE TİC. LTD. ŞTİ.

Address: Köşklü Çeşme Mah.Yeni Bağdat Cad. No:124 Gebze Kocaeli Türkiye

Scope:

Production of Disposable; Sterile Surgical Gowns and Drapes, Nonsterile Gowns and Drapes

Sale of Disposable Sterile Products; (Surgical Gloves, Wooden Tongue Depressor, Surgical Blades, Flowmeter, Infusion (Serum) Set, Urine Bag, Blood Transfusion Set, Blood Lancet)

Sale of Disposable Nonsterile Products; (Examination Gloves, PE Gloves, Mask, Caps, Shoe Covers, Wooden Tongue Depressor, Underpads, Gowns and Drapes, Non-Woven PP Fabrics)

Clauses are excluded: 7.3, 7.5.1.2.2, 7.5.1.2.3, 7.5.3.2.2, 8.2.4.2

Certificate No: NIS 991-01

Issuing Place and Date: ANKARA-31.12.2013

ISO 13485:2003

Quality Management System For Medical Devices

Nissert has verified that the organisation above has established and applies a Quality Management System For Medical Devices. If certification conditions of NİSSERT, and requirements of this Standard are obeyed and surveillance audits are carried out; this certificate is valid until **30.12.2016**

1. Surveillance Audit Visa: 23.12.2014

2. Surveillance Audit Visa: 23.12.2015

Signature
On Behalf of Nissert

You can observe the information of the validation of this certificate from the phone or e-mail address which are below. When surveillance audits are done, stamp is taped on relevant space and signed. Certificates which aren't stamped and signed after the date of surveillance audit are invalid



Address: Gıral 3. Blok No:29 PK 06370
Mecidiyeköy Ankara - Türkiye
Tel: 0312-367 80 08-367 07 87
Fax: 0312-367 00 58 E-mail: nissert@nissert.com



Broche
Broche
Broche
Broche

Broche®

Turgut Reis Mahallesi, Tekstilkent
Koza Plaza B Blok Kat. 3 No.11
Esenler - İSTANBUL / TÜRKİYE

T: +90.212 438 02 42 Pbx
F: +90.212 438 02 48

info@brochemedical.com
www.brochemedical.com



