

AMENDMENT NO. 1 OCTOBER 2024
TO
IS 18266 : 2023 TEXTILES — MEDICAL RESPIRATOR — SPECIFICATION

(Second cover page, foreword, para 4) — Insert the following at the end:

‘For clinical tasks that do not involve exposure to potentially infectious bodily fluids and aerosols; and do not require inward leakage test and fit test, a surgical mask as per IS 16289 may be used rather than a medical respirator. Additionally, in industrial applications, medical respirators should not be used because they lack an exhalation valve and do not meet the requirement of clogging test for coal and dolomite loading.’

(Page 2, clause 4.3) — Insert the following at the end:

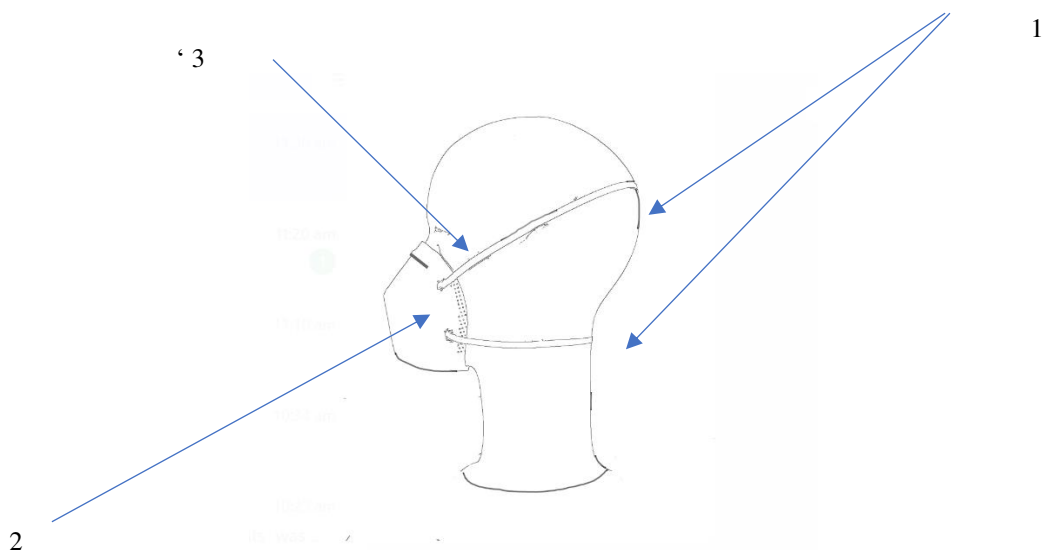


FIG. 1 MEDICAL RESPIRATOR COMPONENTS (FOR GUIDANCE ONLY)

Key

- 1 Head harness
- 2 Filter (fabric layers)
- 3 Nose clip

NOTE — Nose pad and head harness adjuster are optional.’

(Page 2, clause 5.1, second sentence) — Substitute the following for the existing:

‘The medical respirators are classified into two classes based on performance:

- a) IN95 — Filtering out at least 95 percent particles should be use by healthcare personnel (HCP) during all health care setting; and
- b) IN99 — Filtering out at least 99 percent particles should be use by healthcare personnel (HCP) during high-risk situation or for improved fit factor.’

Price Group 1

Amendment No. 1 to IS 18266 : 2023

(Page 3, clause 5.1, Table 1, Note 2) — Substitute ‘should’ for ‘shall’ and ‘design’ for ‘designed’.

(Page 4, clause 6.1) — Insert the following at the end:

‘NOTE — ‘Information given from SI No. (e) to (k) shall be legibly marked on each pack of medical respirator.’

(TXD 36)

Publication, BIS, New Delhi