

AMENDMENT NO. 1 JULY 2023
TO
IS 19022 : 2023 MEDICAL TEXTILES — BARRIER FACE COVERING —
SPECIFICATION

(Page 2, clause 6, second sentence) — Substitute the following for the existing:

‘Reusable barrier face coverings shall withstand at least 5 washing and drying cycles when tested using reference washing machine Type A (wash procedure no. 4 N, 40 °C ± 3 °C) or using reference washing machine Type B (wash procedure 4 B, 41 °C ± 3 °C) using reference detergent 2 and drying procedure (as per care instruction) as specified in IS 15370.’

(Page 2, clause 8, third sentence) — Substitute the following for the existing:

‘The laces, elastic strips, fabric tie etc used as fastening mechanism shall withstand a minimum force of 10 N (for single use face covering) or 50 N (for reusable face covering) when subjected to a tensile force for 10 s with the face covering mounted on a dummy head. The schematic diagram for reference is provided as follows:

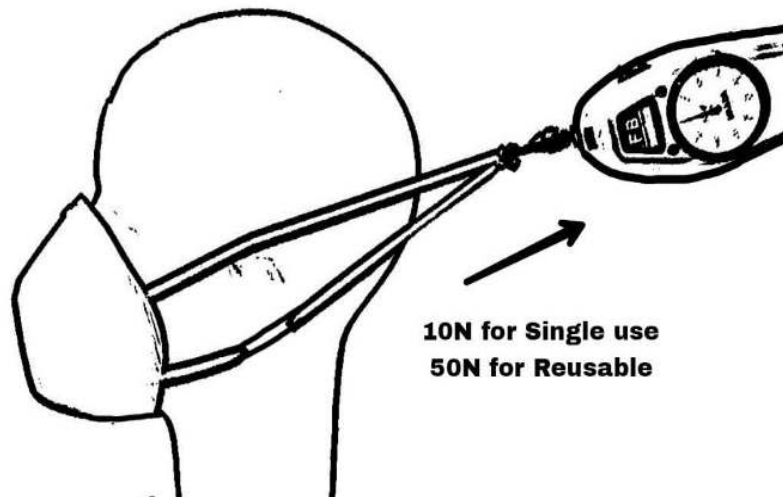


FIG. 1 SCHEMATIC DIAGRAM FOR TIE AND ATTACHMENT STRENGTH TEST (FOR GUIDANCE ONLY)

[Page 3, Table 2, Sl No. (iii)] — Delete.

[Page 3, Table 1, Sl No. (iv)] — Insert the following Note at the end:

‘NOTE — ‘Reusable barrier face coverings shall withstand at least 5 washing and drying cycles when tested using reference washing machine Type A (wash procedure no. 4 N, 40 °C ± 3 °C) or using reference washing machine Type B (wash procedure 4B, 41 °C ± 3 °C) using reference detergent 2 and drying procedure (as per care instruction) as specified in IS 15370.’

[Page 6, Annex B] — Substitute ‘Fig. 2’ for ‘Fig. 1.’

[Page 6, B-2] — Substitute the following for the existing:

‘Suitable breathing resistance test apparatus for measurement of pressure differential equipped with flow meter, pressure gauges etc (such as the apparatus given in Fig. 2).

NOTE —Equivalent automated instruments validated against the test method prescribed may also be used.’

[Page 7, Annex C] — Substitute ‘polystyrene latex’ for ‘latex’.

Amendment No. 1 to IS 19022 : 2023

[Page 7, C-1] — Insert the following Note at the end:

‘NOTE — Instead of aerosol containing suspended polystyrene latex (PSL) spheres, NaCl aerosol may also be used.’

[Page 7, C-2] — Insert the following Note at the end:

‘NOTE — Equivalent automated instruments validated against the test method prescribed may also be used.’