

AMENDMENT NO. 1 MARCH 1984
TO
IS : 5291-1969 SPECIFICATION FOR
TABLES, OPERATION, HYDRAULIC, MAJOR

Alterations

[*Page 5, clause 5.2.1, first and second sentences*] — Substitute the following for the existing sentences.

‘ The head section shall be capable of being raised to 40 to 45° and in its reverse position 120° from the trunk portion. The head section shall be so designed as to be attached on the leg section side in the sitting position. The leg section shall be capable of being raised or lowered to 90° from the trunk so as to enable the table to be used as a chair. A locking mechanism shall be provided at stages of every 15° angle in the sitting position to prevent wobbling of foot section. ’


(*Page 5, clause 5.3, second sentence*) — Substitute the following for the existing sentence:

‘ It shall be operated by a pedal which is so situated as not to obstruct the surgical team while operating in sitting position. ’

[*Page 9, clause 8.1(k)*] — Delete and renumber subsequent item accordingly.


[*Page 9, clause 8.2(f)*] — Substitute the following for the existing item (f):

‘ f) Neuro-surgical attachments as indicated in Fig 1 to 3. ’

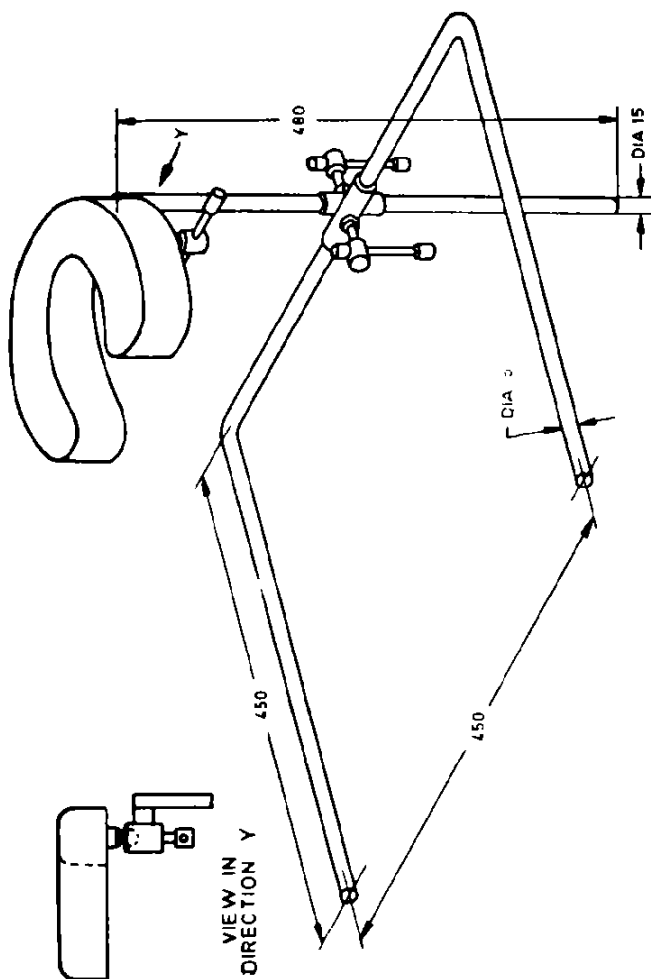


All dimensions in millimetres

FIG 1 NEUROSURGICAL ATTACHMENT FOR SITTING UP POSITION

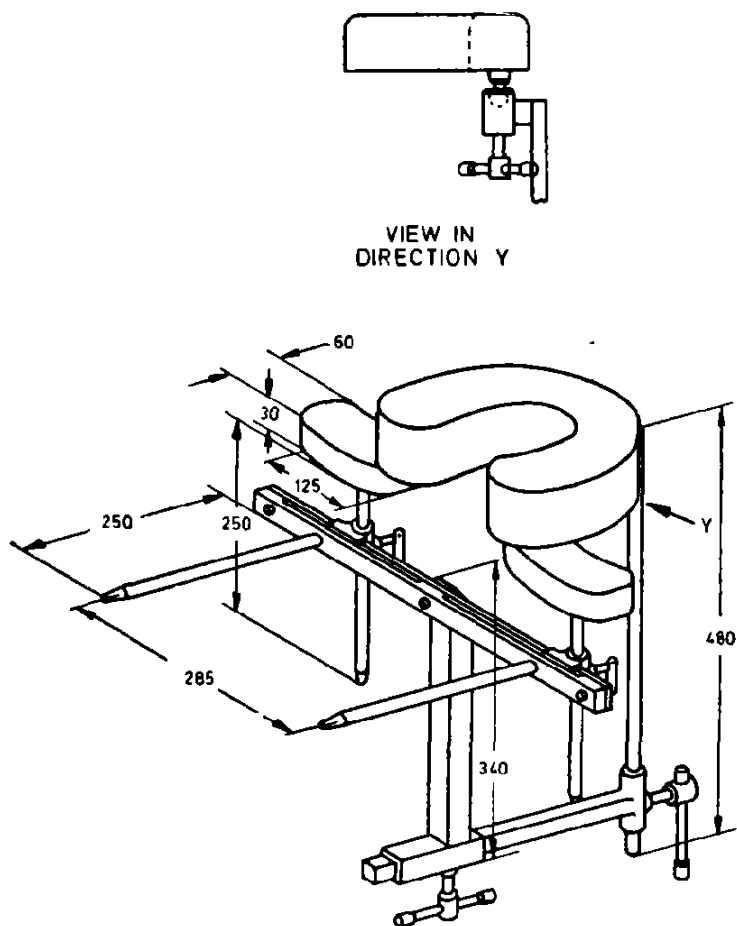

All dimensions in millimetres

FIG. 2 NEUROSURGICAL ATTACHMENT FOR PRONE
POSITION HEAD-REST

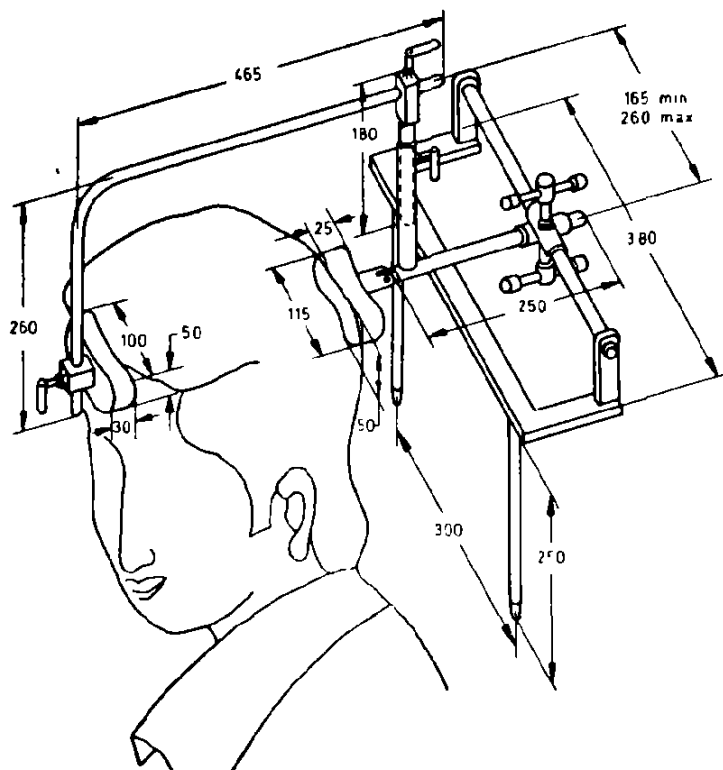

All dimensions in millimetres.

FIG 3 NEUROSURGICAL ATTACHMENT FOR TRIGEMINAL
HEAD-REST

(CPDC 14)