

**AMENDMENT NO. 4 NOVEMBER 2004
TO
IS 3055 (PART 1) : 1994 CLINICAL THERMOMETERS**

PART 1 SOLID STEM TYPE — SPECIFICATION

(*Second Revision*)

(*Page 1, clause 3.1*) — Substitute the following for the existing text:

3.1 For the purpose of this standard, in addition to the definitions given in IS 2627 : 1979, following definitions shall also apply.

3.1.1 *Flat Magnifying Lens* — Thermometer stem glass in which the numerals, graduations and lens lie on the same relative surface.

3.1.2 *Reflecting Stem* — Stem glass containing a coloured stripe along its length in a location that, when reflected on the mercury column, allows greater contrast and enables the column to appear tinted.

3.1.3 *Triangular Magnifying Lenses* — Thermometer stem glass in which the numerals and graduations lie on surfaces, that smoothly merge to form a lens.'

(*Page 1, clause 7.2.1, read with Amendment No. 3*) — Add the following at the end of the text:

"The shape, that is, the cross section of the capillary tube shall be prismatic having a lens form as shown in Fig. 1.'

(*Page 1, clause 7.3.1*) — Insert the following at the beginning of the existing text:

"Thermometer stems are classified as follows (*see* Fig. 1):

- a) Flat magnifying lens,
- b) Triangular reflecting magnifying lens, and
- c) Triangular magnifying lens.'

(*Page 2, clause 7.3.1.1*) — Substitute 'Fig. 2' for 'Fig. 1'.

(*Page 2, clause 7.3.4*) — Substitute 'Fig. 3' for 'Fig. 2'.

Amend No. 4 to IS 3055 (Part 1) : 1994

(Page 2, Table 1) — Inset the following after SI No. (i) and renumber SI No. (ii)as(iii):

'ii) Scale range, °F 94 to 108 or 94 to 110'

(Page 2, Table 1) — Insert the following after SI No. (ii) and and renumber the subsequent SI No.:

'iv) Smallest scale division, °F 0.2'

[Page 2, Table 1, SI No. (iv)] — Substitute '40 to 75' for '40 to 65'.

[Page 2, Table 1, SI No. (v)] — Substitute the following for the existing:

'Thickness of stem - No dimension of the cross section of flat magnifying stems shall be greater than 7.6 mm nor less that 3.6 mm. No dimension of the cross section of triangular stems shall be less than 3.6 mm.'

(Page 3, clause 7.5.5) — Substitute 'Fig. 2' for 'Fig. 1'.

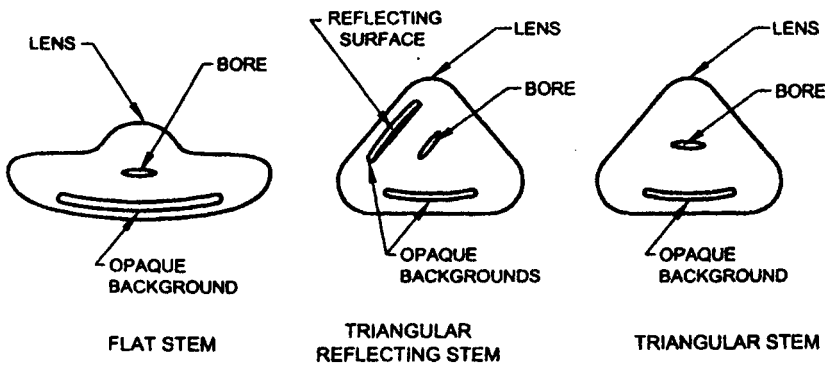


FIG. 1 CROSS SECTION OF MAGNIFYING LENS STEMS

Amend No. 4 to IS 3055 (Part 1) : 1994




FIG. 2 STEM OF CLINICAL THERMOMETER

(CHD 35)