

AMENDMENT NO. 5 DECEMBER 2018
TO
IS 3055 (PART 1) : 1994 CLINICAL THERMOMETERS


PART 1 SOLID STEM TYPE — SPECIFICATION

(Second Revision)


(Page 1, clause 2.1) — Substitute 'IS 2303 (Part 1/Sec 1) : 2012 Grading glass: Part 1 Method of test and classification, Section 1 Hydrolytic resistance of glass grains at 98°C (*second revision*)' for 'IS 2303 (Part 1/Sec 1) : 1994 Method of grading glass for alkalinity: Part 1 Hydrolytic resistance, Section 1 Hydrolytic resistance of glass grains at 98°C — Method of test and classification (*first revision*)'.

[Page 1, clause 7.2.1 (see also Amendment Nos. 3 and 4)] — Substitute the following for the existing clause:

‘7.2.1 The thermometers shall be made from glass tubing conforming to IS 4529 except for ‘stability of bulb tube’ and ‘limit of alkanity’. The shape, that is, the cross section of the capillary tube shall be prismatic having any one of the lens forms as shown in Fig. 1.

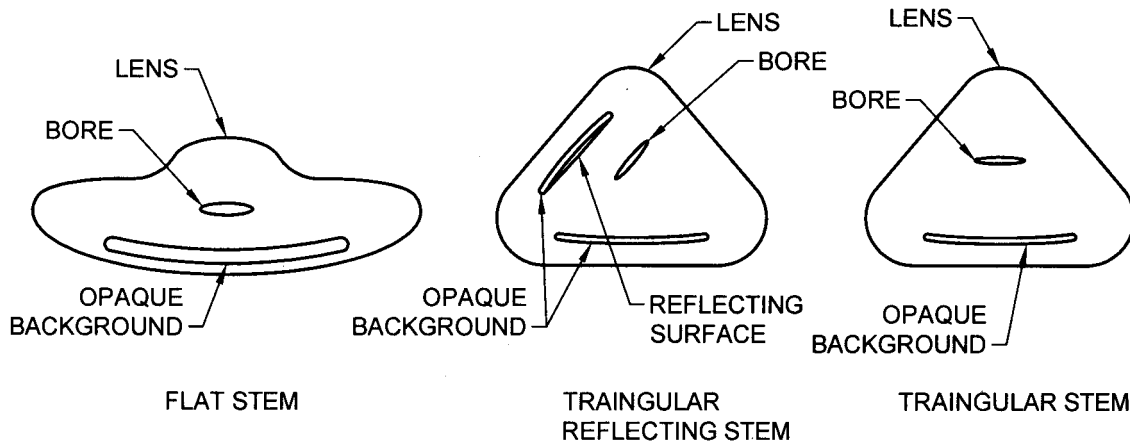

[Page 2, clause 7.3.1.1, Fig. 2 (see also Amendment Nos. 3 and 4)] — Substitute the following figure for the existing:

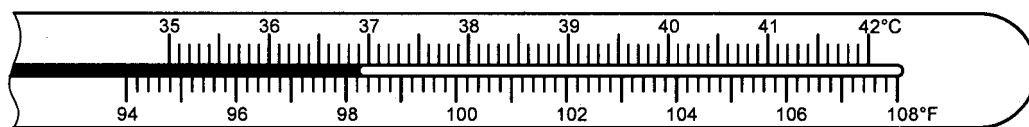

(Page 2, Fig. 2 under clause 7.3.4.1, Caption, read with Amendment No. 4 for clause 7.3.4) — Substitute ‘FIG. 3’ for ‘FIG. 2’.

(Page 2, clause 7.3.4.1, line 1) — Substitute ‘of’ for ‘or’.

(Page 2, clause 7.5.1) — Substitute the following for the existing:

‘7.5.1 The thermometer scale shall be sub-divided in 0.1°C and 0.2°F as shown in Fig. 2.’

[Page 3, clause 7.5.6 (see also Amendment No. 3)] — Substitute ‘Fig. 2’ for ‘Fig. 1’.