

AMENDMENT NO. 1 NOVEMBER 1984
TO
IS : 9459 - 1980 SPECIFICATION FOR APPARATUS
FOR USE IN MEASUREMENT OF LENGTH
CHANGE OF HARDENED CEMENT
PASTE, MORTAR AND CONCRETE

Alterations

(*Page 4, clause 3.1, fifth sentence*) — Substitute the following for the existing matter:

‘ The end of the yoke opposite to the micrometer end of the reference bar shall be provided with an anvil having a cylindrical or conical recess.’


(*Page 4, clause 3.1.1, line 5*) — Substitute ‘ yoke ’ for ‘ frame ’.

(*Page 4, clause 3.2, line 4*) — Substitute ‘ 12 mm ’ for ‘ 20 mm ’.

(*Page 5, Fig. 1*) — Substitute ‘ YOKE ’ for ‘ PILLAR ’.

(*Page 6, Fig. 2*) — Substitute the figure given on page 2 for the existing figure.

[*Page 7, Table 1, col 3, Sl No. (i)*] — Substitute ‘ ISLC 150 or ISMC 150 conforming to IS : 226-1975* ’ for the existing matter.

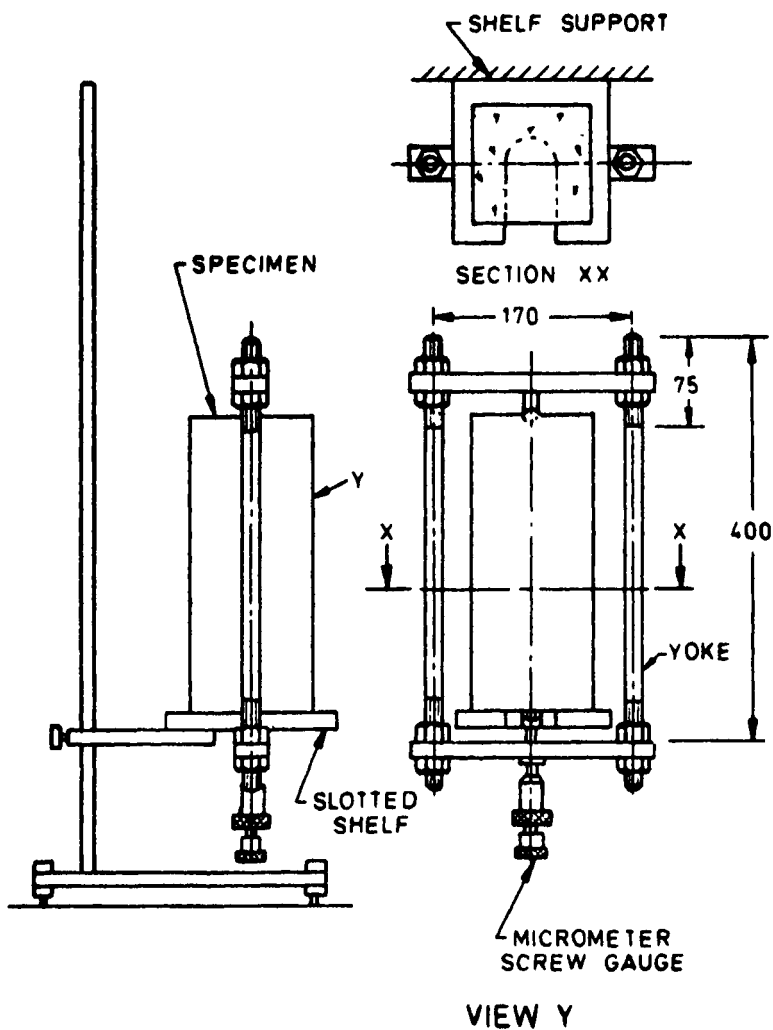

All dimensions in millimetres.

FIG. 2 TYPICAL SET UP FOR DRYING SHRINKAGE AND MOISTURE MOVEMENT TEST ON HEAVY SPECIMEN

(BDO 2)