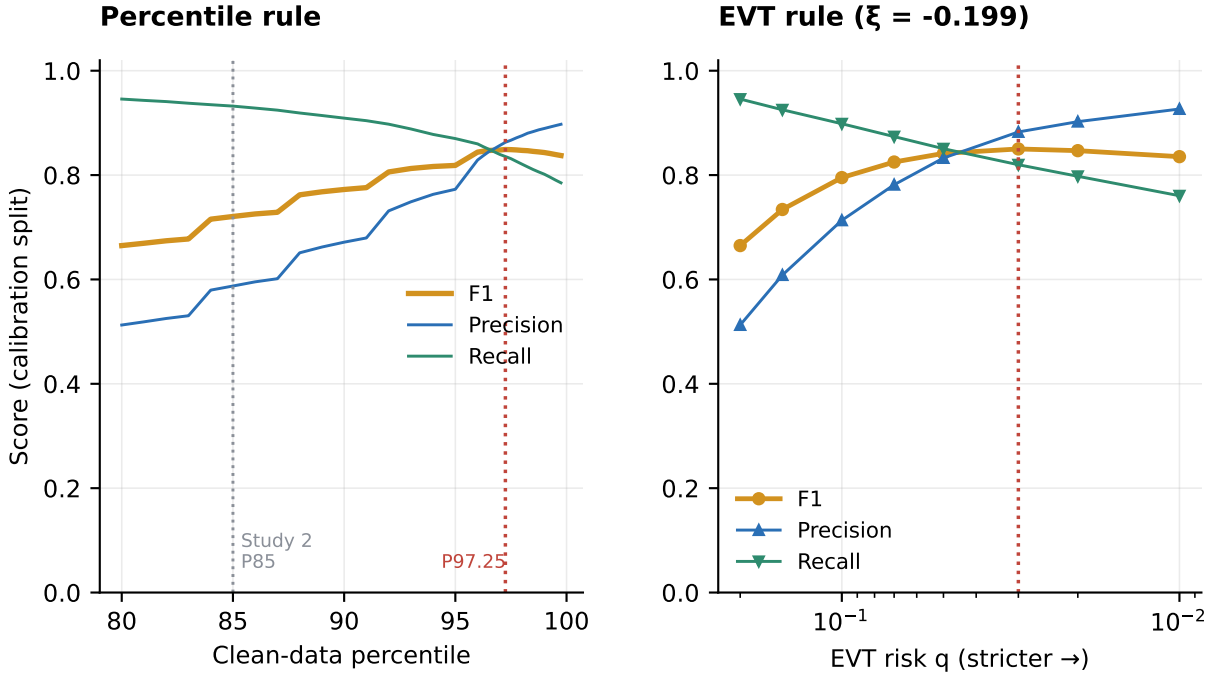Choosing the operating point on clean, held-out calibration data