

# Single Field Analysis

Name: VIJAYA BALAN C.

ID: 160840

Eye: Right

DOB: 25-10-1945

## Central 24-2 Threshold Test

Fixation Monitor: Gaze/Blind Spot

Fixation Target: Central

Fixation Losses: 2/17

False POS Errors: 0 %

False NEG Errors: 25 %

Test Duration: 06:57

Fovea: 31 dB ::

Stimulus: III, White

Background: 31.5 ASB

Strategy: SITA-Standard

Pupil Diameter: 6.8 mm




Visual Acuity: 6/6

RX: +3.25 DS +2.25 DC X 180

Date: 05-06-2018

Time: 9:40 AM

Age: 72

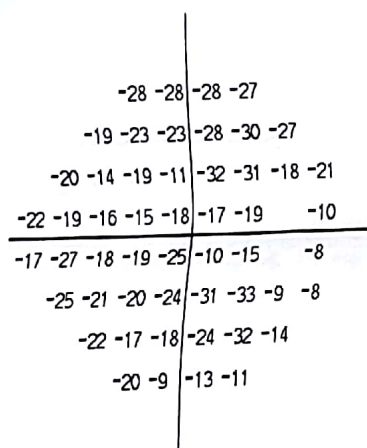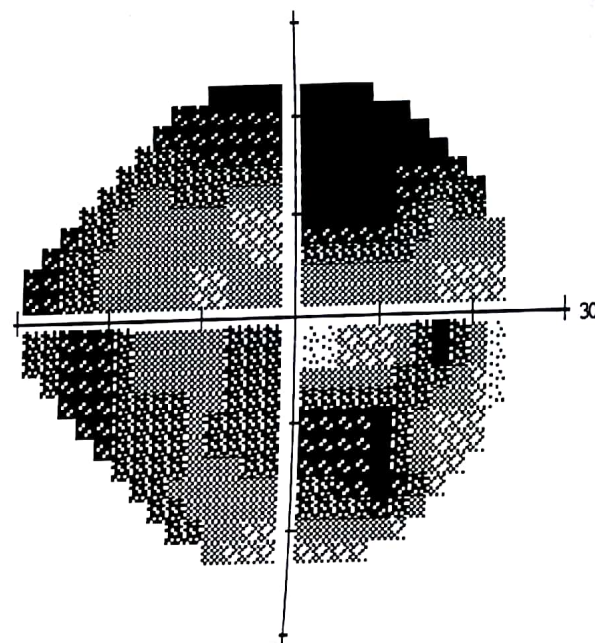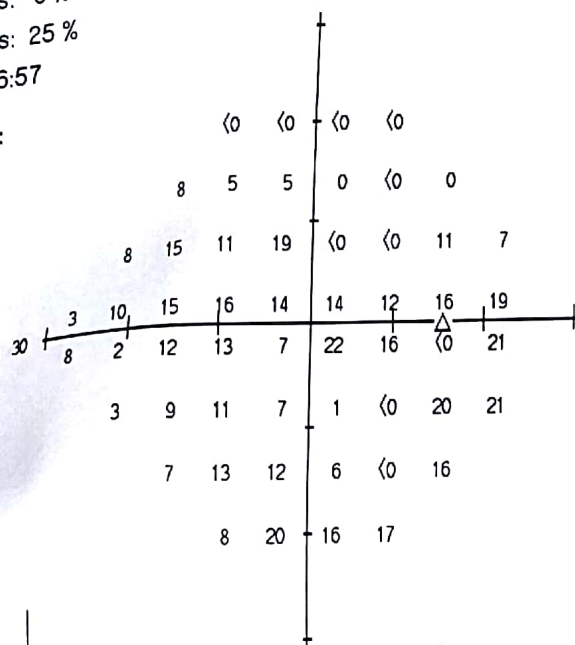

Total Deviation

Pattern Deviation not shown for severely depressed fields. Refer to Total Deviation.


GHT  
Outside normal limits

VFI 34%

MD -20.12 dB P < 0.5%

PSD 7.09 dB P < 0.5%

Pattern Deviation

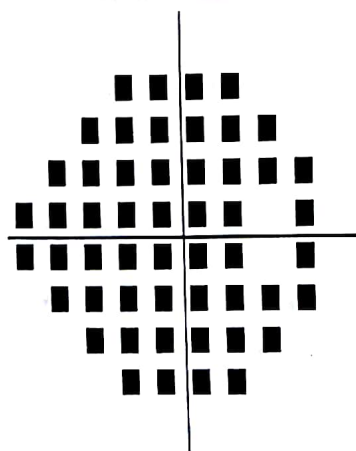

Pattern Deviation not shown for severely depressed fields. Refer to Total Deviation.

:: < 5%

⊗ < 2%

⊗ < 1%

■ < 0.5%

Aravind Eye Hospital  
Thavalakuppam  
Pondicherry