

# Single Field Analysis

Eye: Left

Name: MEENA V.

DOB: 28-04-1985

ID: 1065287

## Central 24-2 Threshold Test

Fixation Monitor: Blind Spot

Fixation Target: Central

Fixation Losses: 0/14

False POS Errors: 10 %

False NEG Errors: 1 %

Test Duration: 04:54

Fovea: 33 dB

Stimulus: III, White

Background: 31.5 ASB

Strategy: SITA-Standard

Pupil Diameter: 3.0 mm




Visual Acuity: 6/6

RX: -2.00 DS DC X


Date: 29-05-2018

Time: 3:28 PM

Age: 33

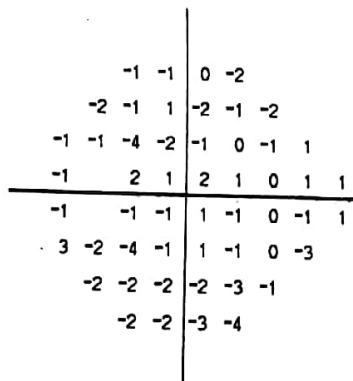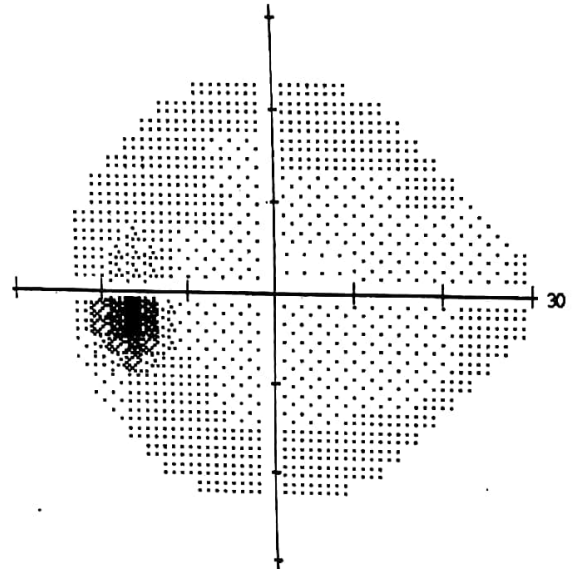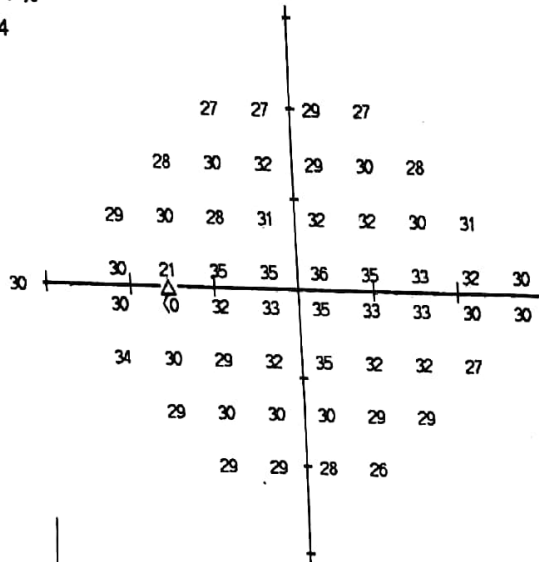

Total Deviation

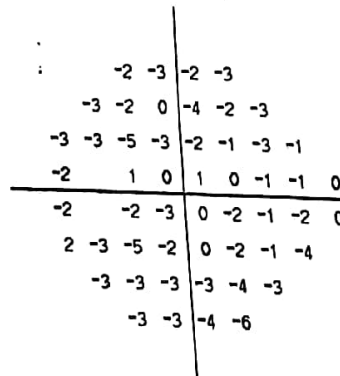

Pattern Deviation



GHT

Within Normal Limits

VFI 99%

MD -0.73 dB

PSD 1.75 dB

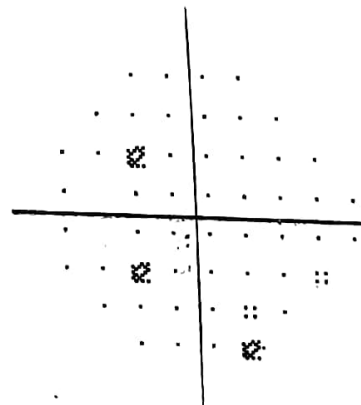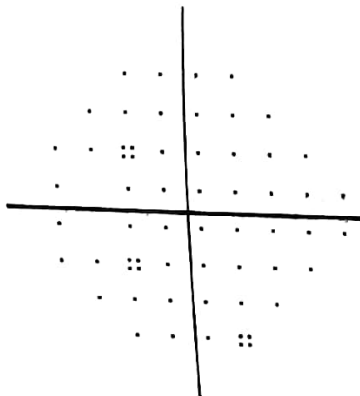

:: < 5%  
 ☼ < 2%  
 ■ < 1%  
 ■ < 0.5%

Aravind Eye Hospital  
Thavalakuppam  
Pondicherry

# Single Field Analysis

Name: MEENA V.

ID: 1065287

Eye: Right

DOB: 28-04-1985

## Central 24-2 Threshold Test

Fixation Monitor: Gaze/Blind Spot

Fixation Target: Central

Fixation Losses: 2/15

False POS Errors: 15 % xx

False NEG Errors: 19 %

Test Duration: 07:31

Stimulus: III, White

Background: 31.5 ASB

Strategy: SITA-Standard

Pupil Diameter: 3.0 mm

Visual Acuity: 6/6



RX: -1.75 DS DC X

Date: 29-05-2018

Time: 3:00 PM


Age: 33

Fovea: 36 dB

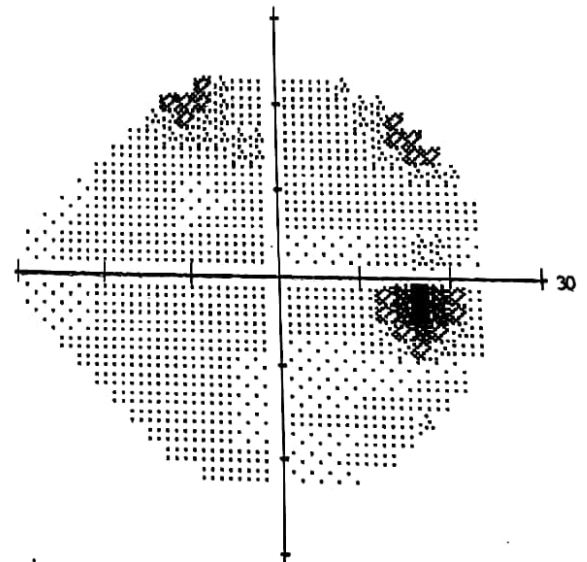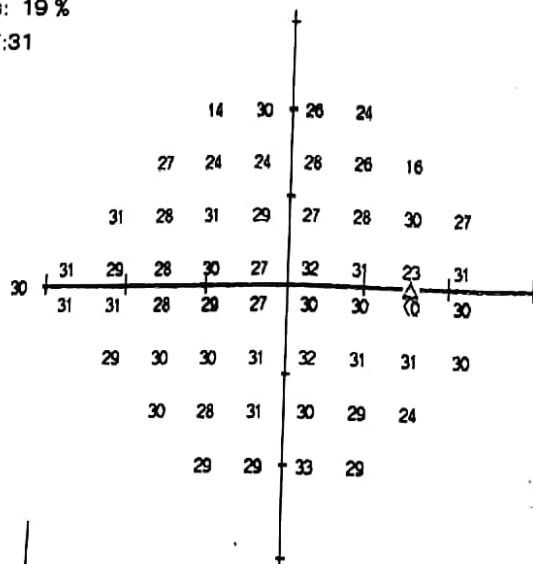

-15	1	-3	-4
-4	-7	-7	-3
1	-3	-2	-4
2	-2	-4	-4
2	0	-4	-5
-1	-2	-3	-3
-1	-3	-1	-2
-1	-1	2	-2

Total Deviation

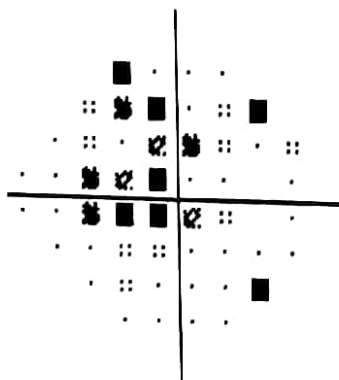

-15	1	-3	-4
-3	-7	-7	-3
1	-3	-2	-4
2	-2	-4	-4
2	0	-4	-5
-1	-2	-3	-3
-1	-3	-1	-2
-1	-1	2	-1

Pattern Deviation



:: < 5%  
 ◻ < 2%  
 ◻ < 1%  
 ■ < 0.5%

\*\*\* Excessive High False Positives \*\*\*

GHT

Outside Normal Limits

VFI 93%

MD -3.15 dB P < 2%

PSD 2.87 dB P < 2%

Aravind Eye Hospital  
 Thavalakuppam  
 Pondicherry