

Single Field Analysis

Name: SRIPRIYA S

ID: 1362201

Central 24-2 Threshold Test

Fixation Monitor: Gaze/Blind Spot

Fixation Target: Central

Fixation Losses: 0/13

False POS Errors: 1 %

False NEG Errors: 0 %

Test Duration: 04:41

Fovea: 36 dB

Stimulus: III, White

Background: 31.5 ASB

Strategy: SITA-Standard

Pupil Diameter: 4.9 mm



Visual Acuity: 6/6

RX: +0.75 DS DC X

Date: 02-06-2018


Time: 12:19 PM

Age: 42

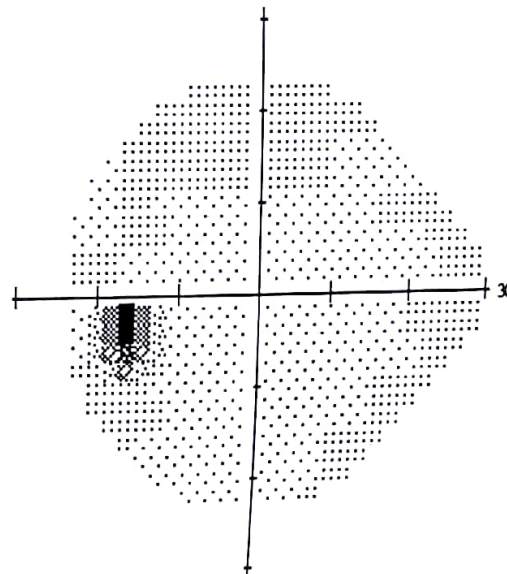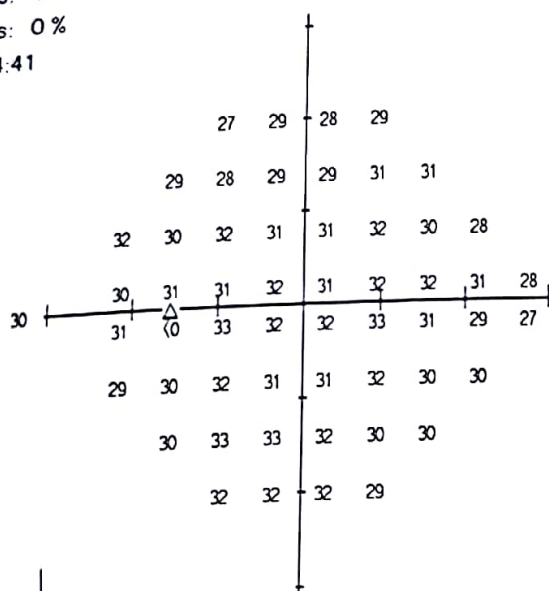


-1	1	0	1
0	-1	-1	-1
2	0	1	-1
0	-1	-1	-2
0	0	-2	-2
-2	-1	0	-2
-1	2	1	0
2	2	2	-1

Total Deviation

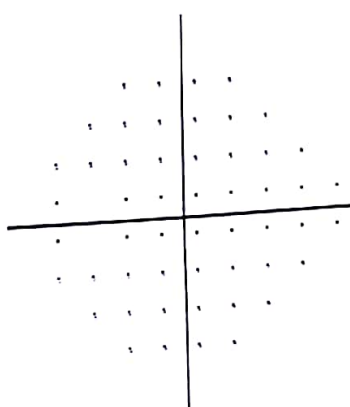

-2	0	-1	0
-1	-2	-2	-2
1	-1	0	-2
-1	-2	-2	-3
-1	-1	-3	-3
-3	-2	-1	-3
-2	1	0	-1
1	1	1	-2

Pattern Deviation

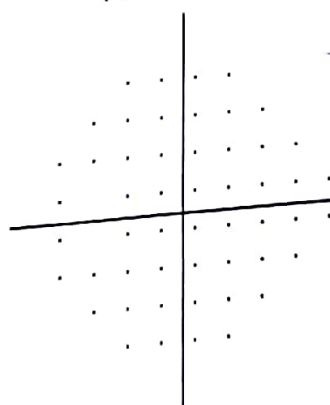

GHT

Within normal limits

VFI 100%

MD -0.50 dB

PSD 1.24 dB

:: < 5%
 ✖ < 2%
 ✖ < 1%
 ■ < 0.5%

Aravind Eye Hospital
Thavalakuppam
Pondicherry

Single Field Analysis

Eye: Right

Name: SRIPRIYA S

DOB: 09-05-1976

ID: 1362201

Central 24-2 Threshold Test

Fixation Monitor: Gaze/Blind Spot

Stimulus: III, White

Pupil Diameter: 5.3 mm

Date: 02-06-2018

Fixation Target: Central

Background: 31.5 ASB

Visual Acuity: 6/6

Time: 12:11 PM

Fixation Losses: 0/14

Strategy: SITA-Standard

RX: +1.25 DS DC X




Age: 42

False POS Errors: 0 %


False NEG Errors: 0 %

Test Duration: 04:12

Fovea: 37 dB

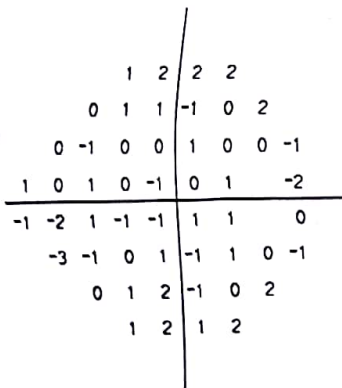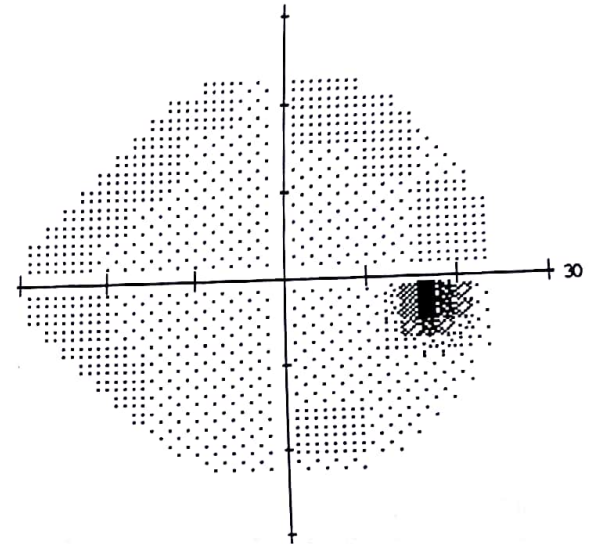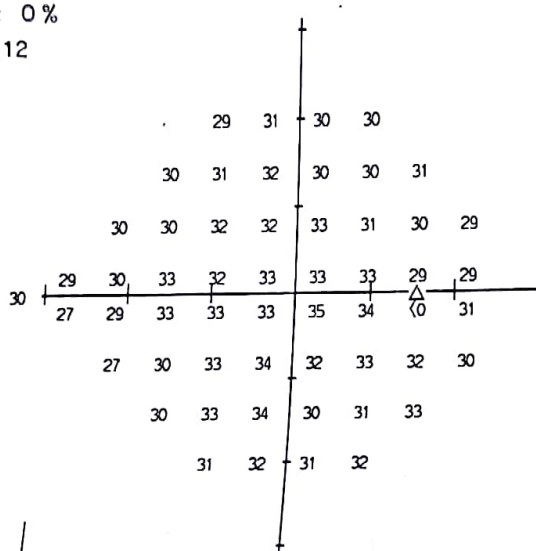

Total Deviation

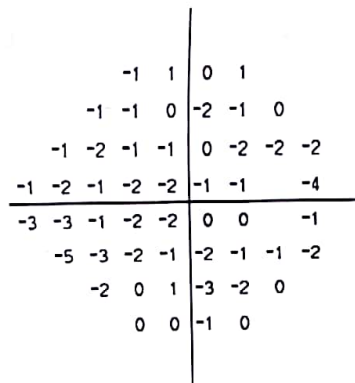

Pattern Deviation

GHT

Within normal limits

VFI 100%

MD +0.25 dB

PSD 1.18 dB

:: < 5%
 ☒ < 2%
 ☒ < 1%
 ■ < 0.5%

Aravind Eye Hospital
 Thavalakuppam
 Pondicherry

