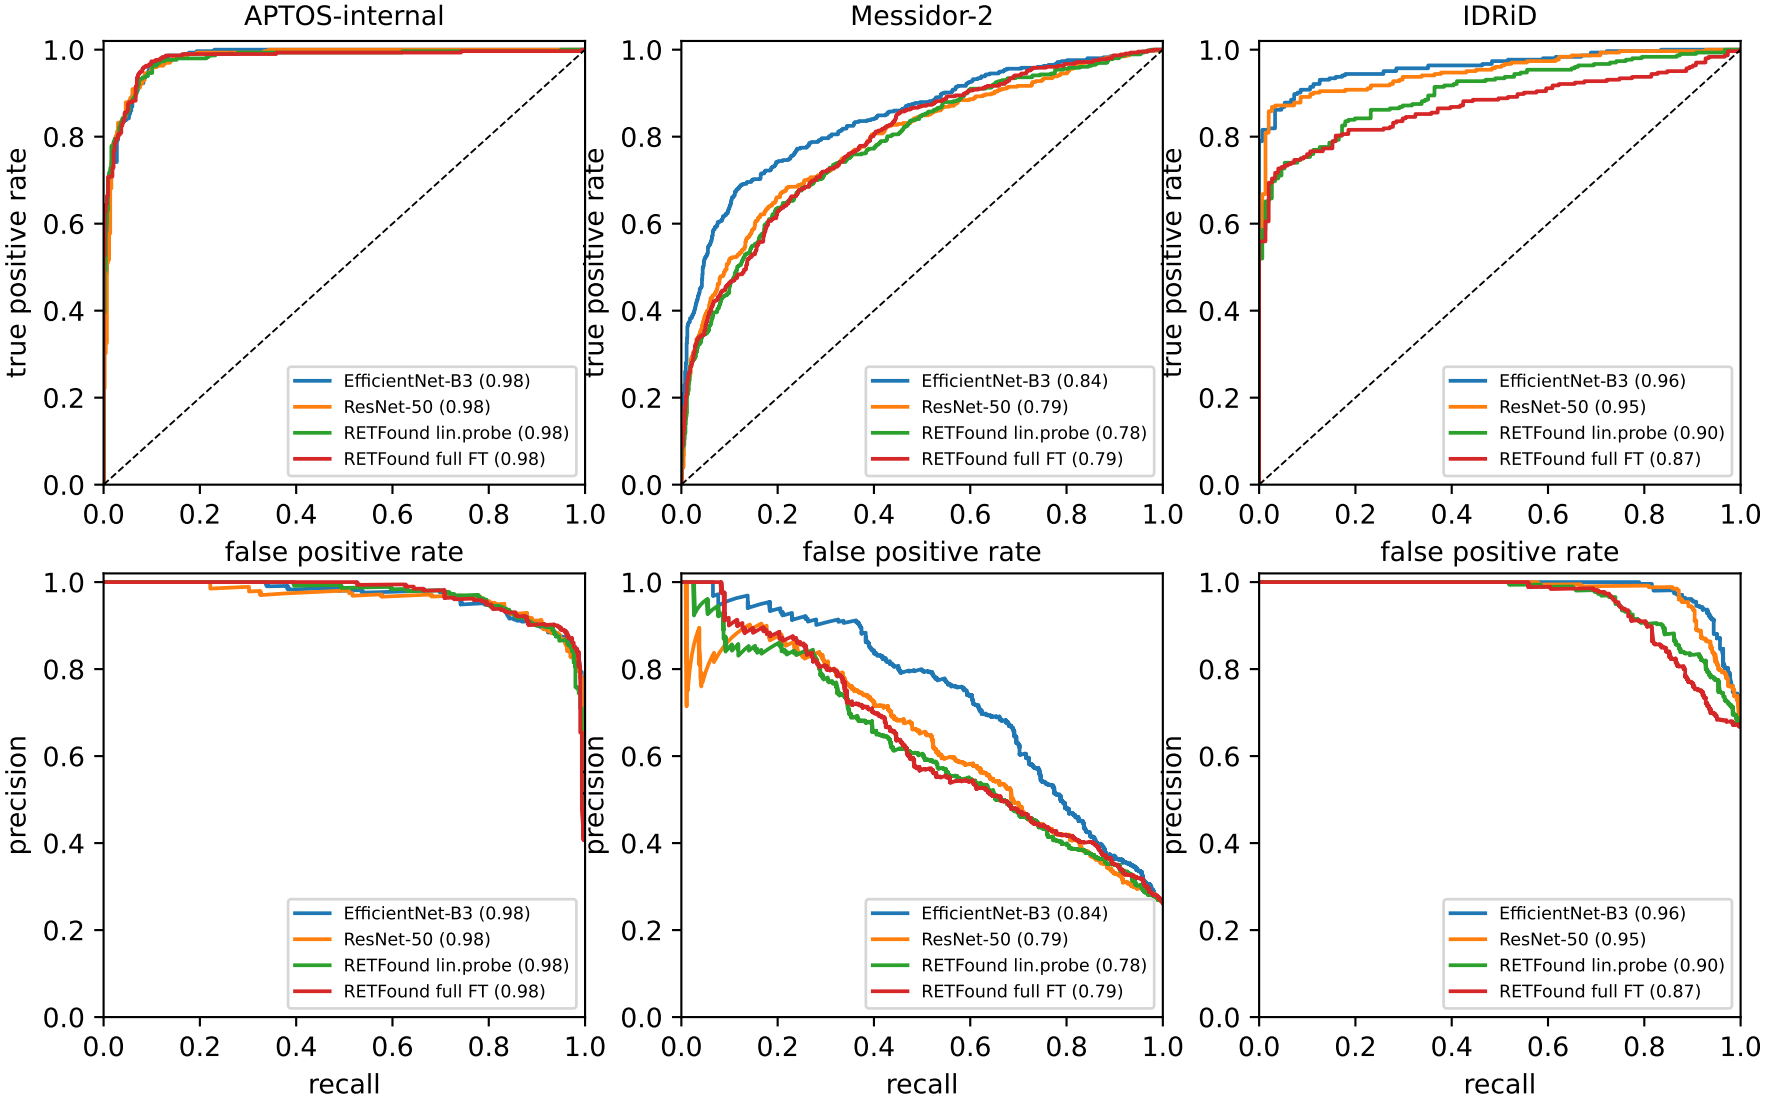

Referable DR (ICDR grade ≥ 2): ROC (top) and precision-recall (bottom); AUROC in legend
APTOS-internal
Messidor-2
IDRiD
true positive rate
false positive rate
precision
recall
EfficientNet-B3 (0.98)
ResNet-50 (0.98)
RETFound lin.probe (0.98)
RETFound full FT (0.98)
EfficientNet-B3 (0.84)
ResNet-50 (0.79)
RETFound lin.probe (0.78)
RETFound full FT (0.79)
EfficientNet-B3 (0.96)
ResNet-50 (0.95)
RETFound lin.probe (0.90)
RETFound full FT (0.87)