



TECHNISCHE
UNIVERSITÄT
WIEN

Project Report

Preliminary research on an electron beam setup for the QUAK experiment

performed at Atominstitut



at Technische Universität Wien
Faculty of Physics

under the supervision of
Assistant Prof. Dr.rer.nat. Philipp Haslinger
and
Projektass.(FWF) Dipl.-Ing. Thomas Weigner

by _____

set date to Eng

Frank Takara Ebel & Alexander Preimesberger

Matrikelnummer: 01429282 & 01427641

Stadionallee 2
1020 Wien

Wien, am 06-01-2021

Contents

1 Short introduction to QUAK	1
2 Cathodic Ray Tube Basics	2
2.1 Underlying Physics	2
2.2 Implementation in the Heerlen D14-363GY	5
2.2.1 The Cathode	7
2.2.2 Cathode Layout	8
3 Cicero Word Generator	10
3.1 Installation of National Instruments drivers	10
3.2 Installation of National Instruments Cards	10
3.3 Configuring Atticus	11
3.3.1 Configure hardware timing / synchronization	11
3.4 Configuration and Basic Usage of Cicero	12
3.4.1 Saving of Settings and Sequences	12
3.4.2 Sequence length limit	12
4 Electron beam setup	13
4.1 Charatarization of a working CRT	13
4.2 High Voltage Power Supply HVPS	14
4.2.1 Ripple measurement	14
4.3 CRT wiring	16
4.4 Heater	17
5 CRT handling	19
5.1 Opening CRTs	19
5.1.1 Rotary tool	19
5.1.2 Wire cutting	19
5.2 Oxygen poisoning	22
6 Vacuum test chamber	25
6.1 First iteration	25
6.1.1 Chamber Setup	25
6.1.2 CRT mounting mechanism	27
6.1.3 Measurement of outgassing	27
6.1.4 Leak test	27

6.2	Second iteration	28
6.2.1	Changes	28
6.2.2	Fastening	28
7	Deflection Electronics	29
7.1	Demands on the setup	29
7.2	Implementation	30
8	Beam Characterization	34
8.1	Aluminum foil	34
8.2	Faraday cup	36
8.3	Deflection frequency	37
9	Next Steps	39
Todo list		40

¹ 1 Short introduction to QUAK

² The goal of QUAK (quantum klystron) is to drive Rabi oscillations between hyperfine
³ levels of the potassium atom using a classical electron beam. Suitable isotopes for this
⁴ experiment are ³⁹K which has a frequency of 461.7 MHz or ⁴¹K with an even lower
⁵ frequency of 254 MHz [[tiecke:potassium-properties](#)]. For this, it is necessary to
⁶ DOPPLER-cool the atoms in a MOT. Once the atoms are trapped, they will be exposed
⁷ to the near-field of the electron beam, which will be spatially modulated with the
⁸ transition frequency. In order to achieve this goal, the beam must allow for a current
⁹ of 100 μ A and a beam waist of 100 μ m.

¹⁰ In our work, we conducted first experiments on how to accomplish an electron beam
¹¹ fulfilling those requirements.

2 Cathodic Ray Tube Basics

This chapter features a quick explanation what a Cathodic Ray Tube (CRT) is and what its main components are. This is followed by a more detailed description on how the individual components are implemented in our used CRT, a Heerlen D14-363GY. The chapter ends with a description of the important characteristics of the CRT and the requirement the theory poses on them.

2.1 Underlying Physics

Wikipedia states: “The cathode-ray tube (CRT) is a vacuum tube that contains one or more electron guns, while a phosphorescent screen and is used to display images. It modulates, accelerates, and deflects electron beam(s) onto the screen to create the images.”

There are three vital components to accomplish this feat: the electron gun, the electron lens and the deflection plates.

Thomas: The electron gun generates free electrons from a cathode material, accelerates them onto an anode and thereby produces an electron beam (see fig. 2.1). One important characteristic in the selection of a cathode material is a low work function. It denotes the amount of energy needed to extract one electron from the material. There are two ways to overcome this energy barrier in an electron gun; one can either apply a strong electric field (“field emission”, “cold cathode”) as seen in fig. 2.2b. Or one can heat the material until some electrons have enough thermal energy to overcome the energy barrier (“thermal emission”, “hot cathode”, fig. 2.2a).

The electron gun generates free electrons from a cathode material, accelerates them onto an anode and thereby produces an electron beam (see fig. 2.1). One important characteristic in the selection of a cathode material is a low work function. It denotes the amount of energy needed to extract one electron from the material. There are two ways to overcome this energy barrier in an electron gun; one can either apply a strong electric field (“field emission”, “cold cathode”) as seen in fig. 2.2b. Or one can heat the material until some electrons have enough thermal energy to overcome the energy barrier (“thermal emission”, “hot cathode”, fig. 2.2a). In the case of the cold

1
2
3
4
5
6

7
8 this section is
9 sometimes co-
10 fusing and al-
11 ready deals w/
12 our CRT

12 you can prob-
13 explain it in
14 own words b-
15 -> maybe bu-
16 wanted some-
17 erally except-
18 definition (for
19 example this
20 includes CRT
21 with multiple
22 electron guns
23 which I was
24 aware of)

25 explain why
26 has to be a s-
27 tip already h-
28 Since it is sh-
29 on the pictur-

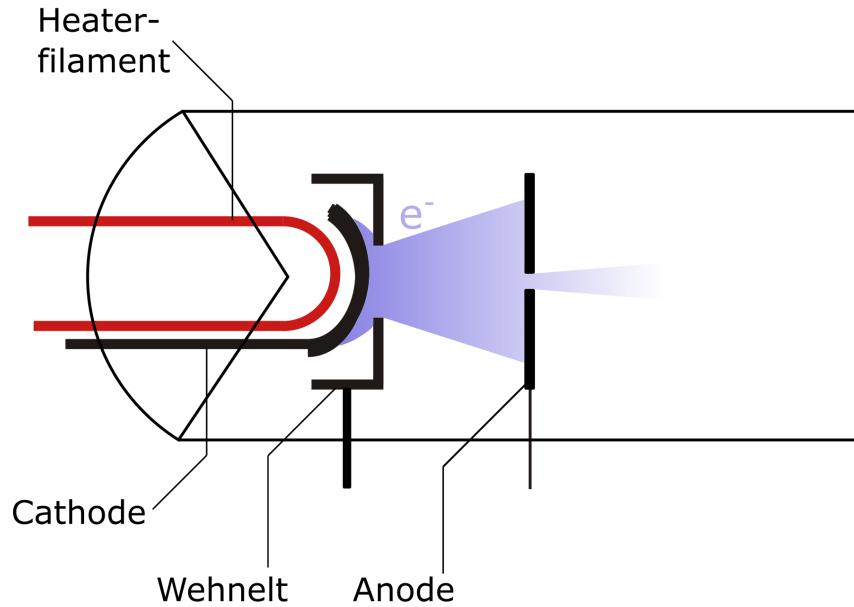



Figure 2.1: Schematic of an electron gun

1 cathode, a cathode with a sharp tip is used, because the electric field on the surface of
 2 a charged conductor is always strongest near sharp points. This causes the electrons
 3 to be emitted from the tip and makes for a very point-like electron source.

4 As our CRT uses a hot cathode, more detail on this will be added later along with
 5 the description of our cathode's design.

6 Normally the cathode itself is covered in beam direction in a so-called Wehnelt
 7 cylinder. Which is a conducting cylinder set to a slightly more negative potential
 8 than the cathode. This part implements two features; firstly it condenses the emitted
 9 electrons, leading to a smaller spot size, i.e. making the cathode a more point-like
 10 electron source. Secondly it enables us to regulate the beam current, the more negative
 11 the Wehnelt potential is, the less electrons are emitted by the electron gun. As we
 12 make the Wehnelt potential more positive, the beam current increases and continues
 13 to rise even after it is more positive than the cathode itself. However, the spot size
 14 gets increased, while the proper beam focus is lost.

15 The electrons, that leave the electron gun, are still divergent and need to be focused.
 16 For our 2 keV electrons an electrostatic lens is used. In the simplest way these are
 17 cylindrically symmetrical pieces of conductor, like a ring or tube, set to an electrical
 18 potential. By combining several of them, one can create the same effect as a combination

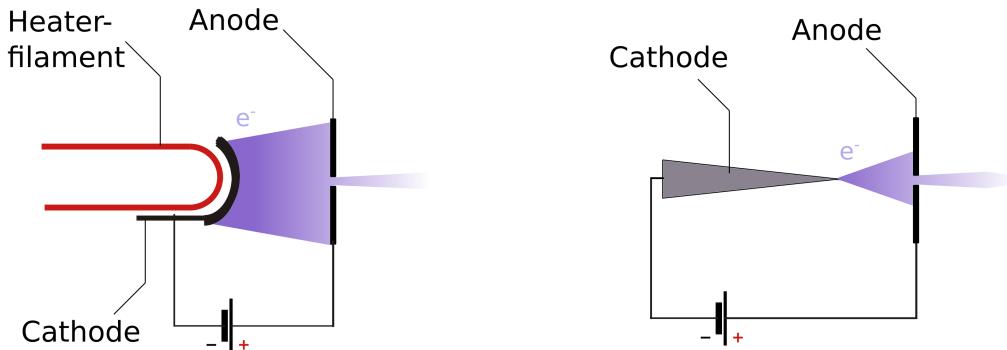

(a) Schematic of a hot cathode

(b) Schematic of field emission cathode

Figure 2.2: Cathode types

of concave and convex lenses ([Demtroeder3]).

The field of this system is simply governed by Laplace's equation in cylindrical coordinates:

$$0 = \frac{1}{r} \frac{\partial \phi}{\partial r} + \frac{\partial^2 \phi}{\partial r^2} + \frac{\partial^2 \phi}{\partial z^2} \quad (2.1)$$

If we take the axis of the beam to be the z-axis, the focal point position in the x-y-plane can be shifted using the two pairs of deflection plates, one for the x- and one for the y-direction. The deflection is achieved by applying a voltage between the two parallel plates. (see: fig. 2.3) By starting with an electron with kinetic energy $e \cdot U_0$ which is accelerated in x-direction by a constant force $e \cdot U_x/d$ over the extent of the plates L , the deflection angle is approximately [Demtroeder3]:

$$\delta \approx \tan(\delta) \approx \frac{U_x \cdot L}{2U_0 \cdot d} \quad (2.2)$$

For the measures of our CRT ($L \approx 10 \text{ cm}$, $d \approx 1 \text{ cm}$, $U_0 \approx 2 \text{ kV}$ and distance to screen $\approx 20 \text{ cm}$) this amounts to a deflection coefficient of around 20 V cm^{-1} , which is quite consistent with the value given in the CRT's manual.

this is a strong statement" -
Yes, too strong
of a statement
actually

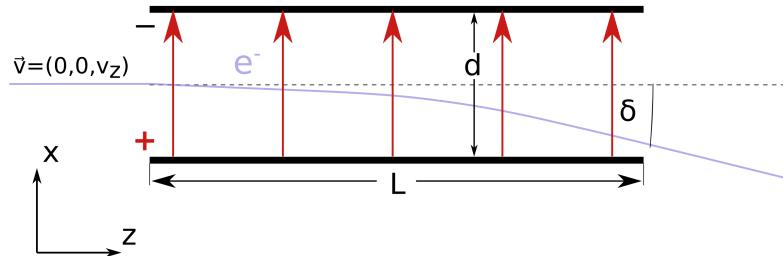


Figure 2.3: Deflection of an electron beam in a constant electrical field

2.2 Implementation in the Heerlen D14-363GY


This section describes the CRT that is used in this project: PDS/CRT Heerlen D14-363GY. Figure 2.4a shows an image of said CRT and fig. 2.4b shows a schematic depiction. The cathode is not visible, as it is fixed inside the Wehnelt cylinder (1), just a few millimeters from the exit of the Wehnelt cylinder the electrons pass through the hole in the anode (2), they gain their full kinetic energy over this short distance. The electrons that go through the hole and enter the electrostatic lens, have 2 keV and therefore move at a speed of approximately $0.08 c$. The electrostatic lenses are realized using three conducting rings (3), that are set to the same potential but have varying radii: Each consecutive ring has a smaller radius than the previous one.

Between the electrostatic lens and the deflection plates, there is another aperture (4), which is internally connected to the anode and is thereby kept at the same potential. In our Setup, the deflection plates are not simply parallel but are shaped like funnels (5,7), between the two pairs of deflection plates, we have the final aperture (6). Its potential can be regulated separately (usually it's on the same potential as the anode)


Finally the beam hits the phosphorous-coated screen which fluoresces on electron impact.

It is connected to the aquadag¹ coating inside the glass envelope and prevents charge building up, that could lead to image distortions. Finally the beam hits the

¹A conductive coating used in CRTs, it consists of graphite particles dispersed in water

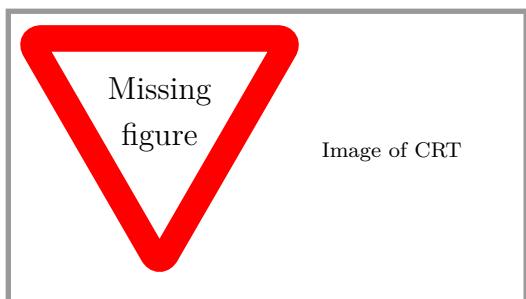

(a) Image picture of the Heerlen D14-363GY

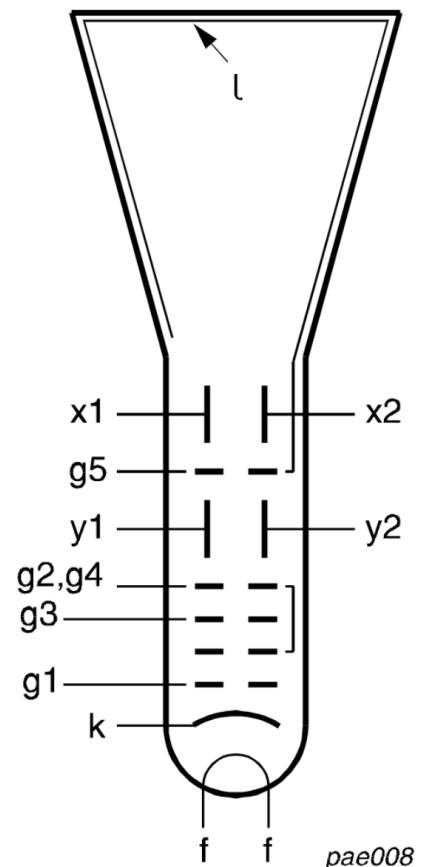

(b) Schematic of the CRT from [D14363GY123-manual]

Figure 2.4

¹ phosphorous-coated screen, which fluoresces on electron impact.

² 2.2.1 The Cathode

³ As already mentioned, we are using a hot cathode, where electrons are thermally excited
⁴ to leave the material. Compared to cold cathodes which work by field emission, this
⁵ leads to a broader energy distribution. For electron microscopy, where a high resolution
⁶ is the goal, this is undesirable, as it leads to some degree of chromatic aberration
⁷ in the electron optics; for our purposes, this should not be a problem. On the other
⁸ hand, hot cathodes normally allow for higher current densities. This is very important
⁹ to QUAK because a high current density allows for a high amplitude of the beam's
¹⁰ dipole radiation and therefore a strong coupling to the potassium atoms. The electron
¹¹ current by thermal emission is described by [Whitaker]:

mention why
is important
done

¹²
$$I = A \cdot T^2 \cdot e^{-b/T} \quad (2.3)$$

¹³ Where b is proportional to the work function of the material, T is temperature and
¹⁴ A is a material-dependent constant. It is clear from this formula, that a low work
¹⁵ function and a high melting point are important characteristics for a good cathode
¹⁶ material.

¹⁷ The cathode from one of our Heerlen D14-363GY-tubes has been removed and
¹⁸ examined with EDX (Energy-dispersive X-ray Spectroscopy). Nickel, barium, and
¹⁹ strontium have been found, which suggests that it is a metal oxide cathode with barium-,
²⁰ strontium-, and possibly aluminum-oxide. This type of cathode is very common in low
²¹ power electron tubes.

²² The "Power Vacuum Tubes Handbook" [Whitaker] describes a typical oxide cathode
²³ as a coating of barium and strontium oxides on a structure made from nickel alloys.
²⁴ Nickel is chosen for its strength and toughness, which it retains even at high temperatures.
²⁵ These cathodes are normally made by coating a case structure with a mixture
²⁶ of barium and strontium carbonates (typically 60 % Ba and 40 % Sr), suspended in a
²⁷ binder material and then baking the structure, causing the carbonates to be reduced
²⁸ to oxides.

²⁹ These metal oxide cathodes normally operate at 700 °C to 820 °C and are capable of
³⁰ average emission densities of 100 mA cm^{-2} to 500 mA cm^{-2} . Higher peak emissions are
³¹ possible for shorter periods of time. As already mentioned, one of the advantages of
³² this type of cathode is its high emission current capability compared to cathodes made
³³ from other materials. Downsides to this cathode type are its greater susceptibility
³⁴ to so-called oxygen poisoning and to ion bombardment. The literature therefore

in our ONEr
are some SE
pictures of t
cathode

recommends to avoid prolonged exposure to oxygen. Oxygen poisoning is the process
in which oxygen adsorbs onto the cathode and increases its work function, effectively
reducing the ability to emit electrons.

Also the material from the oxide cathode will evaporate during the tube's lifetime
and will travel to other parts of the tube, adsorbing to electron optics parts and turning
them into additional emitters. The literature ([Whitaker]) therefore, also advises
against exceeding the design value for the heater voltage, as this reduces the lifetime
of the cathode significantly. CRTs are typically designed to operate for ten years or
longer. For QUAK however, a shorter lifetime is acceptable. Therefore during the
course of our project, we did drive the cathode with higher heater voltages on various
occasions in order to increase the available beam current. We still don't know exactly
how fast the degradation due to this effect proceeds; further research is necessary.

2.2.2 Cathode Layout

Figure 2.5 shows how metal oxide cathodes for CRTs typically look. The depiction
agrees very well with the layout of our cathode. On the image we see the cathode
cylinder, which corresponds to the nickel support structure mentioned above. It is
shaped into a cup, in which the heater filament (shaped into a coil) is inserted. The
oxide disk, from where the electrons are emitted, is baked onto the top of the cathode
cylinder. The cathode cylinder is mounted on an isolating support structure and
inserted into the Wehnelt cylinder, which is called "grid cup" in the drawing.

2 Cathodic Ray Tube Basics

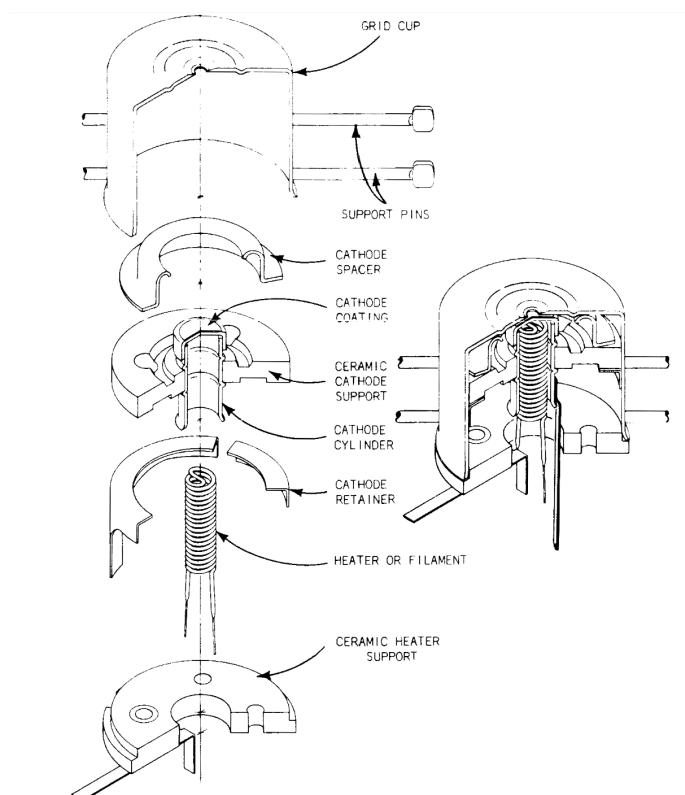


Figure 2.5: Schematic of the layout of a typical CRT-cathode from [deVere69]

3 Cicero Word Generator

1

This chapter describes the installation and initial setup of Cicero Word Generator [keshet2013distributed] on a PC running Windows 10 with analog and digital cards from National Instruments (NI). The code is freely available on GitHub [akeshet:Github]. This chapter contains only differences, problems, and possible solutions encountered when Cicero was installed for the PC ‘Fritz Fantom’ which will be used for the QuaK experiment. It is therefore advised to use the technical and user manual [akeshet:manual] in conjunction.

2
3
4
5
6
7
8

3.1 Installation of National Instruments drivers

9

Before setting up the Cicero Word Generator, it is necessary to install the newest .NET Framework [microsoft:download.net] from Microsoft. Then NI drivers, NI-DAQmx (version 9.3), NI-VISA (newest version), and NI-4888.2 (newest version) should be downloaded from the National Instruments website [ni:drivers] and installed. When installing the NI drivers it is possible to get an ‘Runtime Error!’. In this case it is necessary to set the Regional format settings of Windows 10 to ‘English (United States)’ [ni:runtimerror].

10
11
12
13
14
15
16

3.2 Installation of National Instruments Cards

17

After installation of the necessary drivers, the physical cards can be inserted in the PCIe slots on the motherboard. On ‘Fritz Fantom’ the digital card (NI PCIe-6537B) was installed on PCIe bus 3 while the analog cards (NI PCIe-6738) were installed on PCIe bus 4 and 5.

18
19
20
21

¹ 3.3 Configuring Atticus

² After installation of the NI cards, Atticus should be launched for the first time and
³ closed without changing any settings. After this, the NI-DAQmx drivers should be
⁴ updated to the newest version. If version 9.3 was not used when launching Atticus
⁵ in this step, it could result in an error. After this, “Configuring Atticus” on the user
⁶ manual can be followed. The **Server Name** was set to ‘Fritz_Fantom’. **Dev1** to **Dev3**
⁷ were set in the same ascending order as the physical installation on the motherboard.

⁸ 3.3.1 Configure hardware timing / synchronization

⁹ For synchronization, a **Shared Sample Clock** was used with **Dev1** being the master
¹⁰ card. The settings are summarized in table 3.1 and table 3.2. **Dev3** follows the same
¹¹ settings as **Dev2** except ‘SampleClockExternalSource’ was set to ‘/Dev3/RTSI7’. The
¹² ‘SampleClockRate’ is set to 350 kHz since this is the fastest rate with all 32 analog
¹³ channels active. It is possible to raise this to 1 MHz by only using 8 channels (1 channel
¹⁴ per bank).

Table 3.1: Settings for **Dev1**.

Setting	Value
MasterTimebaseSource	
MySampleClockSource	DerivedFromMaster
SampleClockRate	350000
UsingVariablenamebase	False
SoftTriggerLast	True
StartTriggerType	SoftwareTrigger

Table 3.2: Settings for **Dev2**.

Setting	Value
MasterTimebaseSource	
MySampleClockSource	External
SampleClockExternalSource	/Dev2/RTSI7
SampleClockRate	350000
UsingVariablenamebase	False
SoftTriggerLast	False
StartTriggerType	SoftwareTrigger

3.4 Configuration and Basic Usage of Cicero

After setting up the Atticus server, Cicero can be configured. In step 3.c. it is necessary to write the full IP address and not ‘localhost’.

3.4.1 Saving of Settings and Sequences

The ‘SettingsData’ of the Server Atticus are saved in C:\Users\confetti\Documents\Atticus\SettingsData while the ‘SequenceData’ of Cicero are saved in C:\Users\confetti\Documents\Cicero\SequenceData.

3.4.2 Sequence length limit

The duration of a sequence is limited to $2^{32}/(16 * 32 * 350 \text{ kHz}) = 23.967 \text{ s}$ coming from a 32-bit application, 16 bit per channel, 32 channels in a NI PCIe-6738 card, and 350 kHz clock rate.

¹ 4 Electron beam setup

² 4.1 Charatarization of a working CRT

³ HAMEG HM507 oscilloscopes [HM507-manual] were used for testing purposes which
⁴ contain a D14-363GY/123[D14363GY123-manual] CRT. Although it only has a
⁵ bandwidth of 0 MHz to 50 MHz, which is not sufficient to reach the hyperfine splitting
⁶ frequency of 461.7 MHz for ³⁹K[tiecke:potassium-properties] (or 254 MHz for ⁴¹K),
⁷ it was used nevertheless because of its simple construction and availability. The back
⁸ pin arrangement is shown in fig. 4.1.

⁹ The voltages and currents of the necessary pins to drive the CRT were measured
¹⁰ using a 2.5 kV probe with a voltage divider of 100:1 and are summarized in table 4.1. It
¹¹ was not possible to measure pin g3 directly. Therefore a HVPS (section 4.2) was used
¹² to set a voltage and the beam diameter was observed. The best focus was achieved
¹³ with the value written in the table. The voltage offset of x-, and y-plates was not
¹⁴ possible to measure directly, since it varies with time to draw the necessary image on
¹⁵ the phosphor screen. The given values are the mean of the minimum and maximum
¹⁶ measured voltage. The deflection coefficient is summarized in table 4.2.

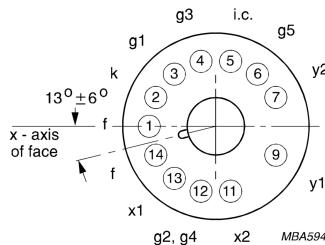


Figure 4.1: Pin arrangement, bottom view from [D14363GY123-manual]

Table 4.1: D14-363GY/123 CRT pin measurements

number	pin	voltage/V	current/ μ A
1	f	-1.99×10^3	86.6×10^3
2	k	-2.00×10^3	-7.6
3	g1	-2.03×10^3	0
4	g3	-1.813×10^3	0
5	i.c.	71.7	0.1
6	g5	64.0	7.2
7	y2	78	-
9	y1	78	-
11	x2	96	-
12	g2, g4	71.0	0
13	x1	96	-
14	f	-1.97×10^3	-86.2×10^3

Table 4.2: D14-363GY/123 deflection coefficient from [D14363GY123-manual]

horizontal	M_x	19 V/cm
vertical	M_y	11.5 V/cm

4.2 High Voltage Power Supply HVPS

To produce high dc voltages to drive the CRT, four HCP 14-6500 power supplies [fug-hcp-manual] were used. They were named ‘HVPS 1’ to ‘HVPS 4’ and can provide up to 2 mA at ± 6.5 kV. To connect the output to the CRT pins, BNC cables were refitted with a save high voltage (SHV) connector on one side while on the other end the BNC connector was kept (fig. 4.2). A 6 kV probe was used to obtain the breakdown voltage, which is around 3 kV caused by the coaxial cable which was not built do sustain high voltages.

4.2.1 Ripple measurement

Each power supply was measured for its ripple with a set voltage of 2 kV. A 2.5 kV probe (attenuation ratio 100:1) was connected to an oscilloscope set to ac coupling with a timescale of 1 ms. To get the electronic noise of the oscilloscope itself, the probe was shorted and the noise measured. A picture of a measurement is shown in fig. 4.3 with the values summarized in table 4.3. As can be seen, the ripple is very close to the noise level and can not really be distinguished.

4 Electron beam setup

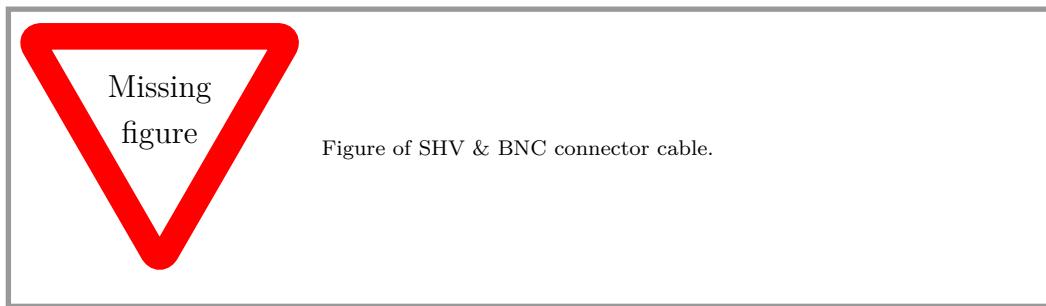


Figure 4.2: Coaxial cable with SHV and BNC connector.

Table 4.3: HVPS ripple

device	ripple/mV
short	116
HVPS 1	136
HVPS 2	138
HVPS 3	194
HVPS 4	204

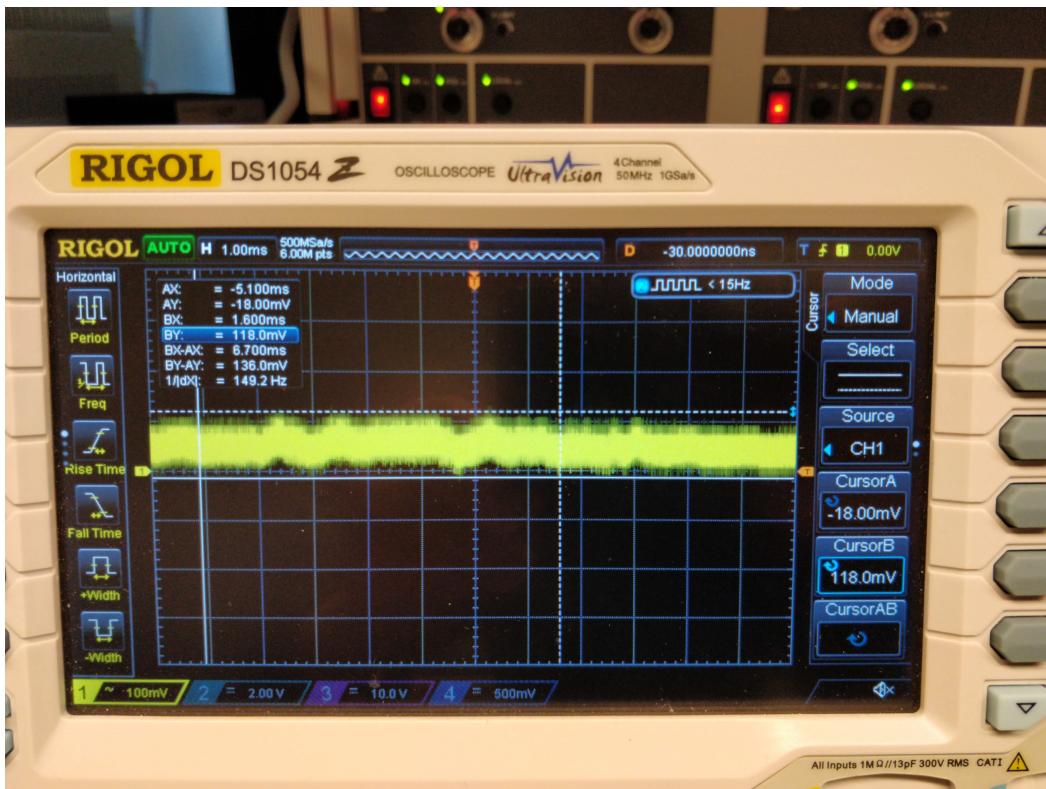


Figure 4.3: Measurement of HVPS ripple.

4.3 CRT wiring

A schematic of the supplied power is shown in fig. 4.4. The pin i.c. stands for internally connected and is wired to pin g2, g4. A small ac or dc voltage is necessary to drive the heater filament f. This part of the setup is explained in section 4.4.



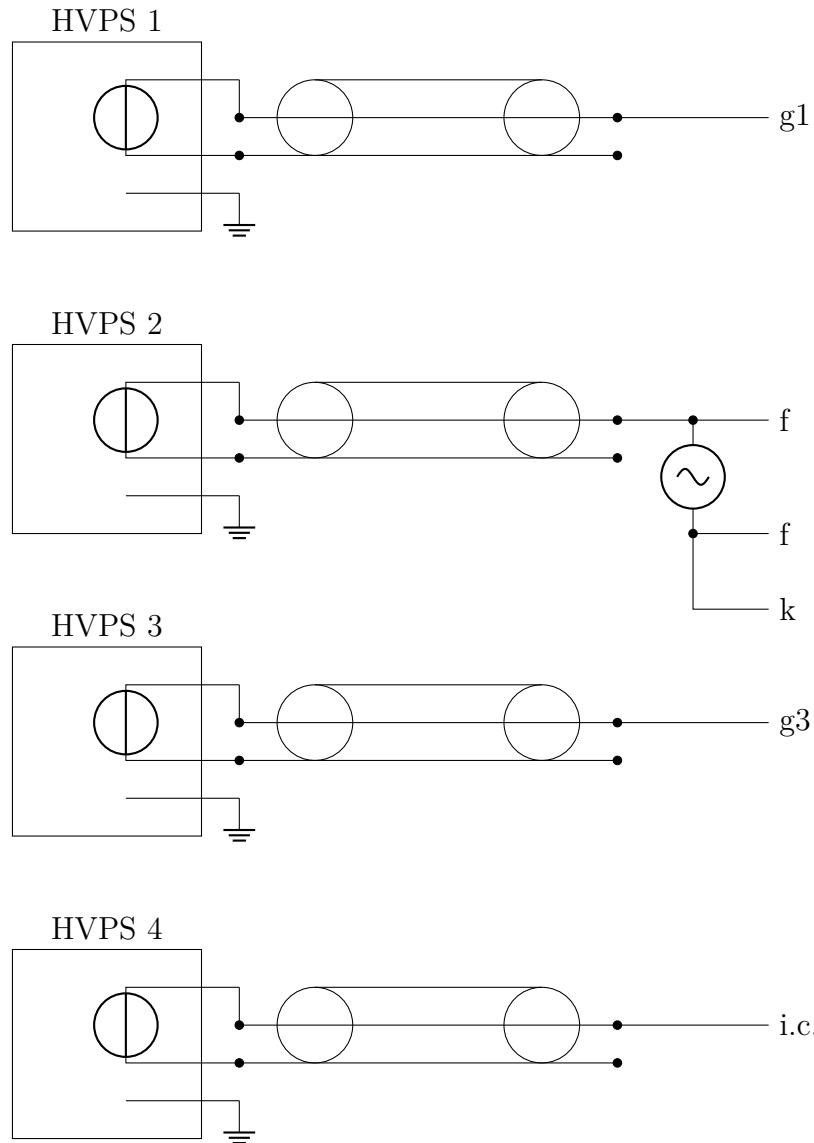


Figure 4.4: Schematics of supplying CRT pins with power.

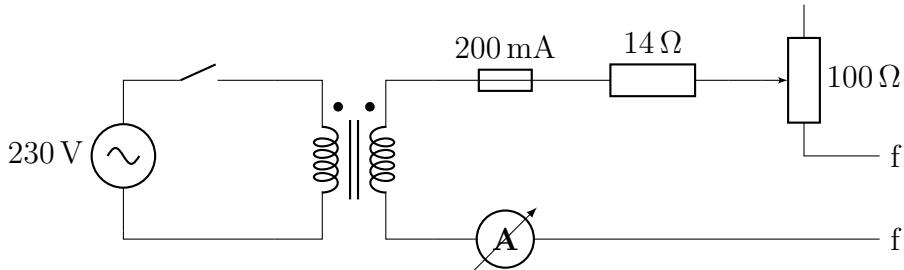

(a) Circuit diagram of filament power supply.

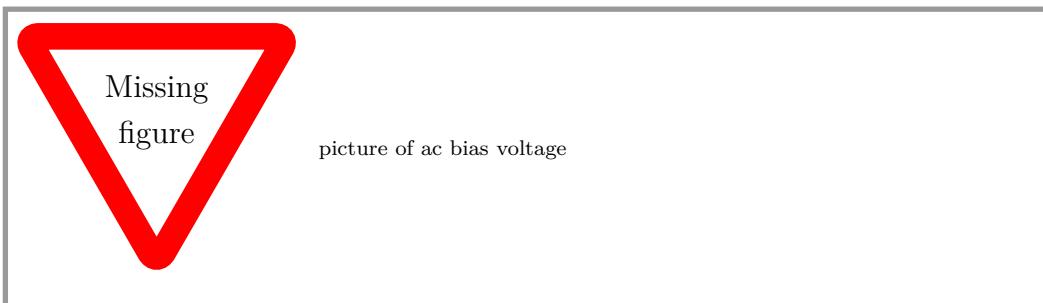

(b) Picture of built filament power supply.

Figure 4.5: AC power supply used to heat the filament with a -2 kV bias voltage.

check if really 14Ω or if it event exists

¹ 4.4 Heater

² The heater provides an adjustable ac voltage, which is used to regulate the temperature
³ of the cathode. In the cold state, the heater filament has a an electrical resistance
⁴ of approximately 15Ω , when the filament is hot, this value rises to 90Ω . The normal
⁵ heater voltage for the D14-363GY/123 during operation is 6.0 V to 6.6 V according to
⁶ [D14363GY123-manual]. Our ac-power supply (shown in figure 4.5) consists of an
⁷ isolation transformer (from grid voltage to 12 V), its primary and secondary circuits
⁸ are isolated up to 4 kV [DS44231-DataSheet]. The power supply has two banana
⁹ plug sockets to connect to the heater filament. It is connected to the transformer
¹⁰ in series with a 100Ω potentiometer. Using the full resistance, there is a voltage of
¹¹ approximately 5.7 V applied to the heater filament, by lowering the resistance this value
¹² can goes up to nearly the full voltage of the transformer. The current running through
¹³ the filament is measured with an integrated ampere meter [ACA-20PC-manual],
¹⁴ that measures currents up to 2 A with mA accuracy.

¹⁵ At the beginning of operation it is recommendable to set the maximum resistance
¹⁶ and slowly increase the current to the desired value once the filament is heated up.

4 Electron beam setup

As the resistance of the cold filament is significantly lower, high onset currents could
¹
otherwise damage it.
²

¹ 5 CRT handling

² 5.1 Opening CRTs

³ In order to have a free electron beam in the experimental setup, to hit a cold ^{39}K , it
⁴ is necessary to cut open the CRT. This section explains the different methods which
⁵ were tried and which resulted in clean and easy cuts. All slices were made in a glove
⁶ box filled with nitrogen gas (fig. 5.1) to reduce oxygen poisoning of the cathode.

⁷ 5.1.1 Rotary tool

⁸ First, a small hole was drilled in the center of the CRT pins to pressurize the CRT
⁹ with nitrogen. Then a diamond wheel attached to a rotary tool was used to cut the
¹⁰ glass. This method was tried twice, but did not work well, as the method produced a
¹¹ lot of glass dust, which adhered to the electron optics. Another obstacle is the plastic
¹² box, since it is not fully transparent and therefore made more difficult to see inside.

¹³ 5.1.2 Wire cutting

¹⁴ Higher success was achieved by cutting the glass with a heated wire. Two wires were
¹⁵ put through the glove box, each ending in a ring terminal. A small height adjustable
¹⁶ stage was built out of optic element mounts (fig. 5.2) in which the CRT was put
¹⁷ vertically and looped by an 0.25 mm steel wire (Fe 70/Cr 25/Al 5). It is important to
¹⁸ keep a small gap in the loop to avoid an electrical short. Therefore two notches were
¹⁹ made in which the wire was fixed.

²⁰ The assembly was put inside the glove box, which was subsequently filled with
²¹ nitrogen. A current of approximately 2 A to 2.5 A was used to heat the thin wire which
²² resulted in a breaking point inside the CRT glass. This method does not require a
²³ CRT pressurization before the cut. In order to not destroy a device by mistake, this
²⁴ procedure was first extensively tested on drinking glasses.

5 CRT handling



Figure 5.1: Glovebox filled with nitrogen gas to open CRTs.

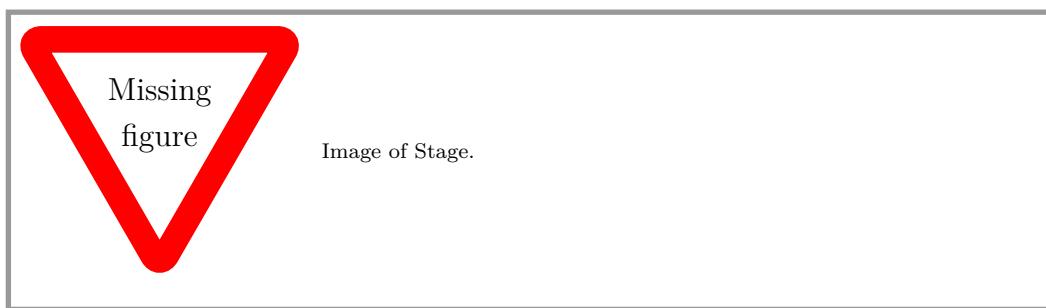


Figure 5.2: Stage to cut CRT with wire.

5.2 Oxygen poisoning

As mentioned in chapter 2 it is paramount to avoid contact of the cathode with oxygen. Therefore tests with a broken CRT were made to test on how well it can be isolated from air.

The first experiment consisted of filling a drinking glass put upside-down with helium and putting a lighter after a set amount of time. If the fire goes off, it means that oxygen did not get inside. This was tested successfully from 0.5 min to 10 min.

Next, plastic wrap was put on top of the glass filled with nitrogen by a rubber band. The glass was put with the open side up from 3 min to 10 min after which it was turned upside down and the foil was removed. A lighter was put inside and the flame went out again.

To improve the precision, a He leak tester was used. For the first two tests, one plastic foil and one rubber band were used; for the third test three foils and two rubber bands; and for the last test an aluminum foil was hot glued on the CRT to seal it. The measurement locations are shown in fig. 5.3. For the glued seal, leakage was measured on the whole circumference. In table 5.1 ‘glue avg’ denotes the average leak rate of this measurement while ‘glue max’ describes the highest value. A seal with rubber band and clear foil tend to higher leakage. Based on these measurements it is recommended to use glued aluminum. But care needs to be taken in order ensure that the whole CRT is sealed since even a small leak can result in a rate around an order of magnitude above the background.

5 CRT handling

Table 5.1: He leak test.

location	leak rate/(10 ⁻⁵ mbar l/s)
1 plastic foil, 1 rubber band	
background	8
plastic foil	20
He gas cylinder	200
1 plastic foil, 1 rubber band	
background	7
plastic foil	20
rubber band	40
3 foils, 2 rubber bands	
background	20
plastic foil	30
rubber band	70
1 aluminum foil, hot glue	
background	6
glue avg	7
glue max	60
aluminum foil	8

5 CRT handling



(a) plastic foil



(b) rubber band



(c) glue



(d) aluminum

Figure 5.3: Measurement locations of He leakage.

¹ 6 Vacuum test chamber

² In order to be able to fit the CRT screen, CF160 flanges were chosen for the test
³ chamber. At one point during testing, major changes were made which will be explained
⁴ in section [6.2](#).

⁶ 6.1 First iteration

⁷ A 3D render of the chamber is shown in (fig. [6.1](#)). Without a CRT installed, it was
⁸ possible to reach a pressure of 6.8×10^{-7} mbar. With a CRT installed inside, the lowest
⁹ achieved pressure was 2.0×10^{-6} mbar. It was not possible to reach a lower pressure
¹⁰ due to outgassing.

¹¹ 6.1.1 Chamber Setup

¹² The center piece consists of a 6-way cross with view ports at the front and bottom.
¹³ A valve was installed at the back in order to flood the chamber with nitrogen
¹⁴ (AlphagazTMN₂ purity $\geq 99.999\%$) when installing a new CRT to reduce oxygen poi-
¹⁵ soning and avoid water vapor getting into the chamber. On the right side, a HiCube
¹⁶ 300 Eco turbo pump was installed and on the left side a wobble stick was attached
¹⁷ with a wire. A straight CF100 pipe of length 27 cm was installed at the top with a 5
¹⁸ port cluster flange, each being of type CF40.

¹⁹ The center piece consists of a 6-way cross with view ports at the front and bottom.
²⁰ A valve was installed at the back in order to flood the chamber with nitrogen, when
²¹ installing a new CRT to avoid oxygen poisoning. On the right side, a HiCube 80 Eco
²² turbo pump was installed and on the left side a wobble stick was attached with a wire
²³. A straight CF100 pipe was installed at the top with a 5 port cluster flange, each
²⁴ being of type CF40.

²⁵ In the middle port, a Thyscont pressure gauge was installed. On the left, a 19
²⁶ pin MIL 19 C connector was installed to supply the necessary voltages to the CRT.
²⁷ Two flanges were equipped with four BNC feedthroughs each. One of them was used

explain more in detail what is the purpose of the chamber the two iterations are not really important built this chapter rather about the function operation of chamber over time due to outgassing the pressure improved

water vapor getting into the chamber

explain in connection of the rendering; this makes it easier if necessary; can get more renderings

pure nitrogen name?

AlphagazTM
1 N₂ purity
 $\geq 99.999\%$

water vapor getting into the chamber

length=27cm

Thyscont ex model is in note

6 Vacuum test chamber

to connect the x-, and y-plates, while the other connected to the wobble stick and aluminum foil at the CRT screen. Further explanation will be given in chapter 8. The last port was capped off by a blank flange.

In the middle port, a VSH pressure gauge was installed. On the left, a 19 pin connector was installed to supply the necessary voltages to the CRT. Two flanges were equipped with four BNC feedthroughs each. One of them was used to connect do the x-, and y-plates, while the other connected to the wobble stick and aluminum foil at the CRT screen. Further explanation will be given in chapter 8. The last port was capped off by a blank flange.

For the inside wires, at first stranded copper cables were used. These were later swapped for Kapton insulated BNC cables. The chamber was sealed by Viton rubber gaskets which were changed to copper gaskets. For the inside wires, standard copper cables were used . The chamber was sealed by rubber gaskets.

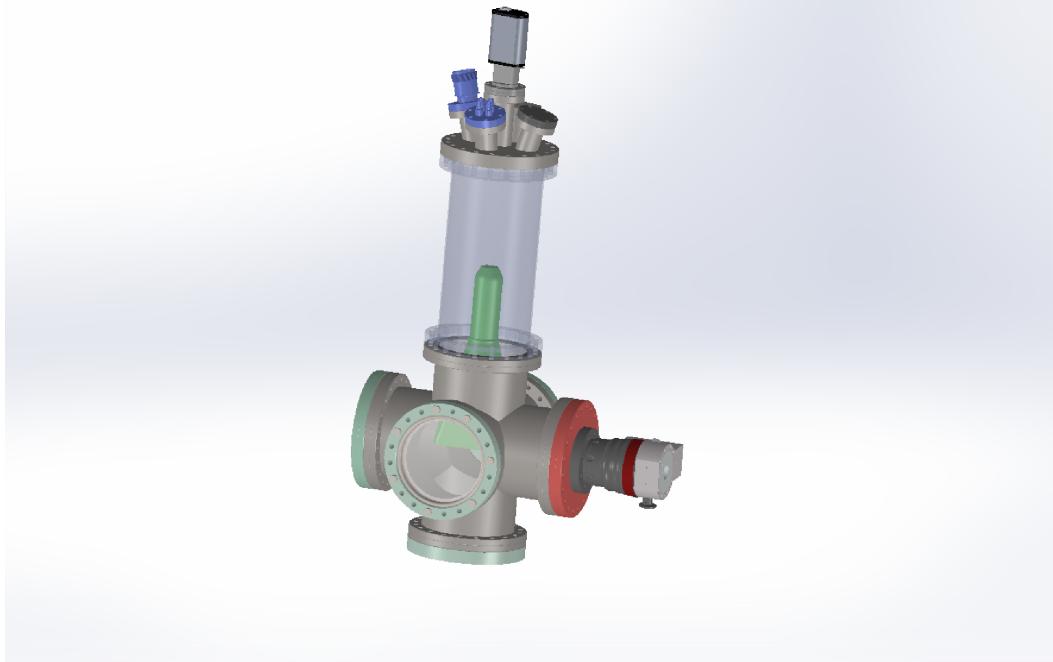


Figure 6.1: 3D rendering of test chamber.

1 6.1.2 CRT mounting mechanism

2 Two M8 rods of length were screwed with a counter nut into the cluster flange. On
3 each, a L shaped aluminum piece was installed between two nuts. These were then
4 connected by a hose clamp, which was used to secure the CRT inside below the cluster
5 flange (fig. 6.2).

6 Two M8 rods of length were drilled into the cluster flange. On each, a L shaped
7 aluminum piece was installed between two nuts. These were then connected by a hose
8 clamp, which was used to secure the CRT inside below the cluster flange (fig. 6.2).

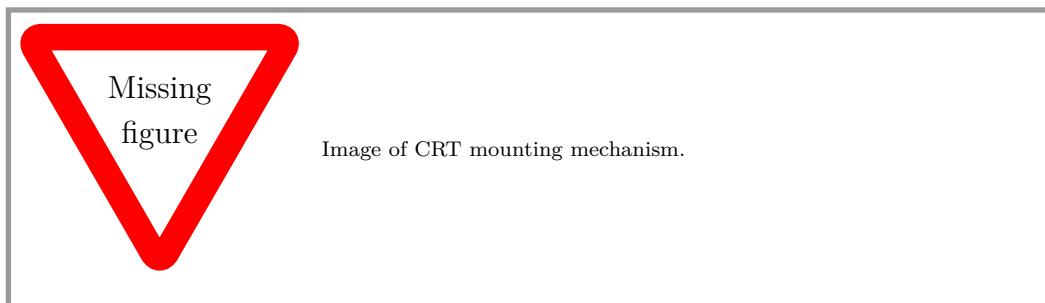


Figure 6.2: Image of CRT mounting mechanism.

9 6.1.3 Measurement of outgassing

10 6.1.4 Leak test

12 Before inserting a CRT for the first time, measurements were made in order to find
13 out how well low pressure could be maintained inside the chamber. First, the chamber
14 was set to a pressure of 10^{-5} mbar after which the pump was turned off. The pressure
15 was measured once a minute for a duration 3 h. This is shown in fig. 6.3.

16 Before inserting a CRT, a leak test was performed. First, the chamber was set to a
17 pressure of 10^{-5} mbar after which the pump was turned off. The pressure was measured
18 once a minute for a duration 3 h. This is shown in fig. 6.3.

rod length? ch
Solid works

rod length? ch
Solid works

screwed / wi
counter nut

in general m
better sectio
titles

this is not so
much of a le
but mainly o
gassing / how
the pressure
sured?

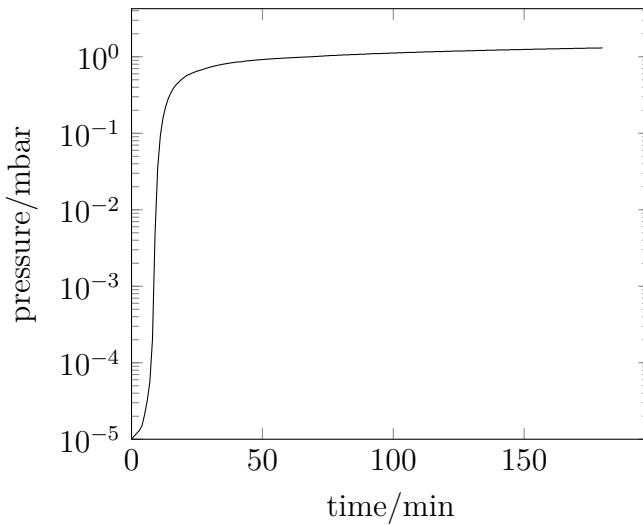


Figure 6.3: Time evolution of pressure inside the test chamber after turning off pump.

6.2 Second iteration

At one point during experimentation, major changes were made to the chamber. Thanks to these, it was possible to reach a pressure of 1.2×10^{-7} mbar.

6.2.1 Changes

First, every rubber gasket was exchanged to a copper one for a better seal, except at the cluster flange, since that spot will be opened and closed the most often. Each copper stranded cable inside was switched to a coaxial one and the mantle was connected to the chamber wall, which was set to ground. A Faraday cup was installed below the wobble stick, to accurately measure the beam current (further details in section 8.2). The aluminum foil was extended to cover all four sides of the screen.

6.2.2 Fastening

When attaching flanges, it is important to start with a low torque and to fasten opposite screws to prevent too much force on one side of the gasket. For M6 screws, the torque was incrementally set to 6 N m, 10 N m, 15 N m and 20 N m and for M8 screws 8 N m, 16 N m and 25 N m. After finishing every opposite screw pair at a set torque, the procedure was repeated twice before going to a higher torque. This was done in order guarantee a tight and even seal.

¹ 7 Deflection Electronics

² 7.1 Demands on the setup

³ For the QuaK experiment it is paramount to be able to deflect a beam of a sufficient
⁴ current precisely at the right frequency with a sufficiently small bandwidth. As
⁵ previously mentioned, our deflection system simply consists of two pairs of parallel
⁶ plates between which a voltage is applied. Controlling this voltage allows us to control
⁷ the deflection of the beam. Various aspects are important here (illustrated in fig. 7.1):

⁸ **Offset:** Although the deflection of the beam is controlled by the voltage between the
⁹ plates, it is necessary to be able to set their mean potential as well. During
¹⁰ normal operation this offset voltage is at 96 V for the x-direction and at 78 V for
¹¹ the y-direction. These offsets are necessary to keep the beam focused.

¹² **Amplitude:** The deflection coefficients in the x and y planes are 19 V cm^{-1} and
¹³ 11.5 V cm^{-1} respectively (see [D14363GY123-manual]). We therefore need
¹⁴ to be able to supply approximately 70 V in order to be able to move the beam in
¹⁵ a large enough area. .

¹⁶ **Frequency:** The final goal is to be able to deflect the beam at the hyperfine splitting
¹⁷ frequency of ^{39}K , which is 461.7 MHz. This is likely to prove impossible with this
¹⁸ CRT-model, observations at the highest frequency we have tried so far will be
¹⁹ discussed in section section 8.3.

²⁰ **Waveform:** Ultimately we want the cold atoms to experience a field that oscillates like
²¹ a sine wave. As a first try it is therefore reasonable to apply a sinusoidal voltage.

²² **Lissajous curves:** Having the ability to control the deflection in both the x- and the
²³ y- axis, allows us to have our beam draw out Lissajous Curves (fig. 7.2). By
²⁴ applying sine waves of equal frequency to both pairs of deflection plates and by
²⁵ being able to control the phase between them we can have the beam oscillate on
²⁶ a straight line or a circle. This allows us to generate either a linearly or circularly
²⁷ polarized field.

Optional: inser
Foto of CRT's
flection plates
fig:DeflectionSe

what happen
when there i
no bias volta
what is the p
pose of it

to achieve w
> good ques
Why did we
that?

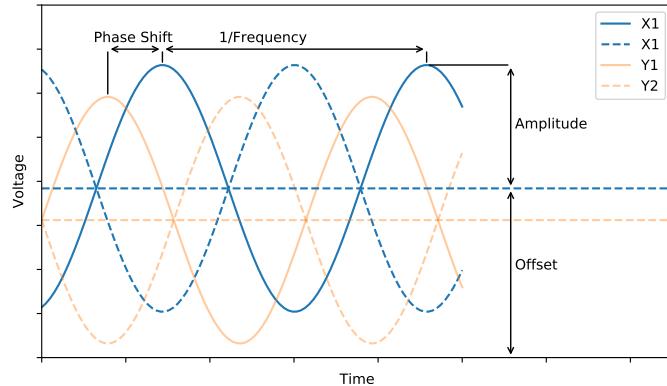


Figure 7.1

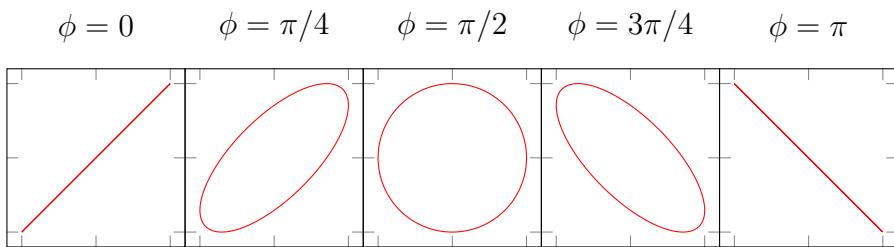


Figure 7.2: Lissajous Curves

7.2 Implementation

A first setup with which we can try to obtain the desired voltages is depicted in fig. 7.3. On the very left we have a signal generator that is capable of producing the right frequency (461.7 MHz) this signal is then split up into an x-, and a y-branch. One of the two branches is connected to a phase shifter, which is able to delay the input signal by up to 200°, allowing us to set any desired phase shift between x-, and y-deflection and to correct for inadvertent delays from the other electronics. Both the x-, and y-signal are then amplified using (amplifier). In the final step, a center tapped transformer allows us to produce voltages for the plates X1 and X2 (or Y1 and Y2 respectively) with a phase shift of exactly 180° between them. By setting the center tap to the desired offset potential, we should get the voltage curves described above. To understand this setup in more detail, it is useful to examine its most important parts more closely:

Amplifier: Up to now we have used the XXX and the YYY amplifier, they amplify the signal by a fixed gain of (How much?) , inputs and outputs can simply be

1
2
3
4
5
6
7
Find out which
plifier
10
11
12
13

14 which model?
15 which model?
Check amplifier
specifications

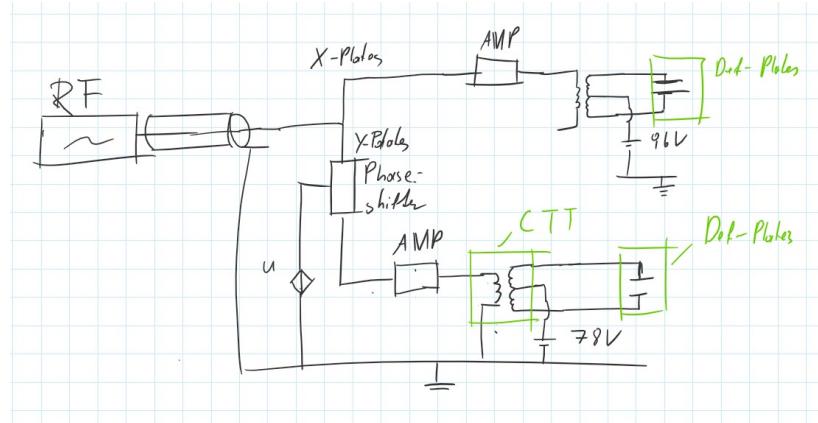


Figure 7.3: Deflection circuit


connected via BNC cables, the amplifier is powered by a linear power supply with a DC voltage of 24 V via two banana plugs in the front. Since we want to control the Lissajous curves shapes (as the deflection coefficients for the x- and y- plates differ), it is desirable to be able to adjust the amplifier gain in future versions of the setup.

Center Tapped Transformer: The center tapped transformer we use is the Mini-Circuits TC8-1G2+ ([TC8-1G2]), a transformer for frequencies between 2 MHz to 500 MHz, with an impedance ratio of 8. Figure 7.6 shows how the center tapped transformer is implemented. The in- and outputs, as well as the bias voltage can be connected via BNC cables. As usual, the shields of all these cables are connected to ground, furthermore they are connected to each other and to the housing. As a safety feature, both outputs X1 and X2 are directly connected to the bias through an arrangement of diodes: Two connections, each with a normal diode and a Zener diode facing in opposite directions. The breakthrough voltage of the Zener diode is 200 V, during normal operation the voltage on it stays below this value and none of the connections let any current through as one of the two diodes is always blocking it. However if one of the plates in the CRT accidentally comes in contact with high voltage, the connection with the appropriately oriented Zener diode opens up, preventing a voltage spike on the center tapped transformer and thereby protecting the electronics connected to its primary circuit. At the point of writing there are still some problems with the behavior of the center tapped transformer, the capacitance of the diodes introduces an undesired phase shift between the two signals. Figure 7.5a shows the circuit's behavior at 465 MHz without its diodes, here the signals are shifted by $120 \text{ ps} \cong 20^\circ = 0.35 \text{ rad}$. Additionally, applying a bias voltage leads to differing amplitudes, as can be seen in fig. 7.5b.


Optional: Go to lab and measure their performance with an Oszi.

Phase Shifter: To control the phase shift between the x- and y-deflection plates, we use a Mini-Circuits [JSPHS-661] phase shifter. This part was put in a housing ([Hammond1455D601RD]) on a separate PCB and can be connected via BNC cables. Figure 7.4a shows how the phase shifter is connected and fig. 7.4b shows the corresponding PCB layout. Note that again the shields of the BNC cables are connected among each other and to the housing. The JSPHS-661+ is designed for frequencies in the range 400 MHz to 600 MHz. By applying a DC voltage of 0 V to 12 V to the bias connector, it is possible to introduce a phase shift of up to 200° to the signal.

(figure)

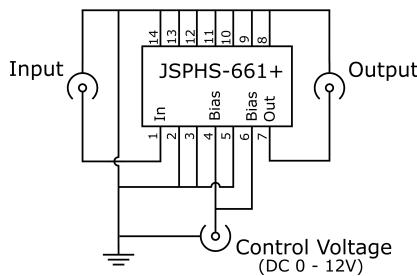

(a) Schematic of phase shifter connections

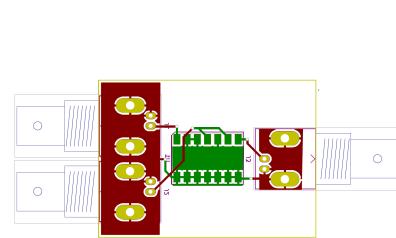


(b) PCB-Layout of the phase shifter

Figure 7.4




(a) Signal of center tapped transformer without diodes, unbiased at 465 MHz

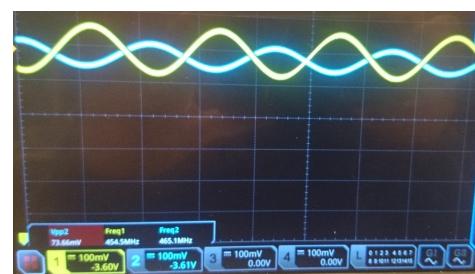

(b) Signal of center tapped transformer without diodes, biased at 465 MHz

Figure 7.5

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
101
102
103
104
105
106
107
108
109
110
111
112
113
114
115
116
117
118
119
120
121
122
123
124
125
126
127
128
129
130
131
132
133
134
135
136
137
138
139
140
141
142
143
144
145
146
147
148
149
150
151
152
153
154
155
156
157
158
159
160
161
162
163
164
165
166
167
168
169
170
171
172
173
174
175
176
177
178
179
180
181
182
183
184
185
186
187
188
189
190
191
192
193
194
195
196
197
198
199
200
201
202
203
204
205
206
207
208
209
210
211
212
213
214
215
216
217
218
219
220
221
222
223
224
225
226
227
228
229
230
231
232
233
234
235
236
237
238
239
240
241
242
243
244
245
246
247
248
249
250
251
252
253
254
255
256
257
258
259
260
261
262
263
264
265
266
267
268
269
270
271
272
273
274
275
276
277
278
279
280
281
282
283
284
285
286
287
288
289
290
291
292
293
294
295
296
297
298
299
300
301
302
303
304
305
306
307
308
309
310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365
366
367
368
369
370
371
372
373
374
375
376
377
378
379
380
381
382
383
384
385
386
387
388
389
390
391
392
393
394
395
396
397
398
399
400
401
402
403
404
405
406
407
408
409
410
411
412
413
414
415
416
417
418
419
420
421
422
423
424
425
426
427
428
429
430
431
432
433
434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465
466
467
468
469
470
471
472
473
474
475
476
477
478
479
480
481
482
483
484
485
486
487
488
489
490
491
492
493
494
495
496
497
498
499
500
501
502
503
504
505
506
507
508
509
510
511
512
513
514
515
516
517
518
519
520
521
522
523
524
525
526
527
528
529
530
531
532
533
534
535
536
537
538
539
540
541
542
543
544
545
546
547
548
549
550
551
552
553
554
555
556
557
558
559
560
561
562
563
564
565
566
567
568
569
570
571
572
573
574
575
576
577
578
579
580
581
582
583
584
585
586
587
588
589
589
590
591
592
593
594
595
596
597
598
599
600
601
602
603
604
605
606
607
608
609
610
611
612
613
614
615
616
617
618
619
620
621
622
623
624
625
626
627
628
629
630
631
632
633
634
635
636
637
638
639
640
641
642
643
644
645
646
647
648
649
650
651
652
653
654
655
656
657
658
659
660
661
662
663
664
665
666
667
668
669
669
670
671
672
673
674
675
676
677
678
679
680
681
682
683
684
685
686
687
688
689
689
690
691
692
693
694
695
696
697
698
699
700
701
702
703
704
705
706
707
708
709
709
710
711
712
713
714
715
716
717
718
719
719
720
721
722
723
724
725
726
727
728
729
729
730
731
732
733
734
735
736
737
738
739
739
740
741
742
743
744
745
746
747
748
749
749
750
751
752
753
754
755
756
757
758
759
759
760
761
762
763
764
765
766
767
768
769
769
770
771
772
773
774
775
776
777
778
779
779
780
781
782
783
784
785
786
787
788
789
789
790
791
792
793
794
795
796
797
798
799
799
800
801
802
803
804
805
806
807
808
809
809
810
811
812
813
814
815
816
817
818
819
819
820
821
822
823
824
825
826
827
828
829
829
830
831
832
833
834
835
836
837
838
839
839
840
841
842
843
844
845
846
847
848
849
849
850
851
852
853
854
855
856
857
858
859
859
860
861
862
863
864
865
866
867
868
869
869
870
871
872
873
874
875
876
877
878
879
879
880
881
882
883
884
885
886
887
888
889
889
890
891
892
893
894
895
896
897
898
899
900
901
902
903
904
905
906
907
908
909
909
910
911
912
913
914
915
916
917
918
919
919
920
921
922
923
924
925
926
927
928
929
929
930
931
932
933
934
935
936
937
938
939
939
940
941
942
943
944
945
946
947
948
949
949
950
951
952
953
954
955
956
957
958
959
959
960
961
962
963
964
965
966
967
968
969
969
970
971
972
973
974
975
976
977
978
979
979
980
981
982
983
984
985
986
987
988
989
989
990
991
992
993
994
995
996
997
998
999
1000
1001
1002
1003
1004
1005
1006
1007
1008
1009
1009
1010
1011
1012
1013
1014
1015
1016
1017
1018
1019
1019
1020
1021
1022
1023
1024
1025
1026
1027
1028
1029
1029
1030
1031
1032
1033
1034
1035
1036
1037
1038
1039
1039
1040
1041
1042
1043
1044
1045
1046
1047
1048
1049
1049
1050
1051
1052
1053
1054
1055
1056
1057
1058
1059
1059
1060
1061
1062
1063
1064
1065
1066
1067
1068
1069
1069
1070
1071
1072
1073
1074
1075
1076
1077
1078
1079
1079
1080
1081
1082
1083
1084
1085
1086
1087
1088
1089
1089
1090
1091
1092
1093
1094
1095
1096
1097
1098
1099
1099
1100
1101
1102
1103
1104
1105
1106
1107
1108
1109
1109
1110
1111
1112
1113
1114
1115
1116
1117
1118
1119
1119
1120
1121
1122
1123
1124
1125
1126
1127
1128
1129
1129
1130
1131
1132
1133
1134
1135
1136
1137
1138
1139
1139
1140
1141
1142
1143
1144
1145
1146
1147
1148
1149
1149
1150
1151
1152
1153
1154
1155
1156
1157
1158
1159
1159
1160
1161
1162
1163
1164
1165
1166
1167
1168
1169
1169
1170
1171
1172
1173
1174
1175
1176
1177
1178
1179
1179
1180
1181
1182
1183
1184
1185
1186
1187
1188
1189
1189
1190
1191
1192
1193
1194
1195
1196
1197
1198
1199
1199
1200
1201
1202
1203
1204
1205
1206
1207
1208
1209
1209
1210
1211
1212
1213
1214
1215
1216
1217
1218
1219
1219
1220
1221
1222
1223
1224
1225
1226
1227
1228
1229
1229
1230
1231
1232
1233
1234
1235
1236
1237
1238
1239
1239
1240
1241
1242
1243
1244
1245
1246
1247
1248
1249
1249
1250
1251
1252
1253
1254
1255
1256
1257
1258
1259
1259
1260
1261
1262
1263
1264
1265
1266
1267
1268
1269
1269
1270
1271
1272
1273
1274
1275
1276
1277
1278
1279
1279
1280
1281
1282
1283
1284
1285
1286
1287
1288
1289
1289
1290
1291
1292
1293
1294
1295
1296
1297
1298
1299
1299
1300
1301
1302
1303
1304
1305
1306
1307
1308
1309
1309
1310
1311
1312
1313
1314
1315
1316
1317
1318
1319
1319
1320
1321
1322
1323
1324
1325
1326
1327
1328
1329
1329
1330
1331
1332
1333
1334
1335
1336
1337
1338
1339
1339
1340
1341
1342
1343
1344
1345
1346
1347
1348
1349
1349
1350
1351
1352
1353
1354
1355
1356
1357
1358
1359
1359
1360
1361
1362
1363
1364
1365
1366
1367
1368
1369
1369
1370
1371
1372
1373
1374
1375
1376
1377
1378
1379
1379
1380
1381
1382
1383
1384
1385
1386
1387
1388
1389
1389
1390
1391
1392
1393
1394
1395
1396
1397
1398
1399
1399
1400
1401
1402
1403
1404
1405
1406
1407
1408
1409
1409
1410
1411
1412
1413
1414
1415
1416
1417
1418
1419
1419
1420
1421
1422
1423
1424
1425
1426
1427
1428
1429
1429
1430
1431
1432
1433
1434
1435
1436
1437
1438
1439
1439
1440
1441
1442
1443
1444
1445
1446
1447
1448
1449
1449
1450
1451
1452
1453
1454
1455
1456
1457
1458
1459
1459
1460
1461
1462
1463
1464
1465
1466
1467
1468
1469
1469
1470
1471
1472
1473
1474
1475
1476
1477
1478
1479
1479
1480
1481
1482
1483
1484
1485
1486
1487
1488
1489
1489
1490
1491
1492
1493
1494
1495
1496
1497
1498
1499
1499
1500
1501
1502
1503
1504
1505
1506
1507
1508
1509
1509
1510
1511
1512
1513
1514
1515
1516
1517
1518
1519
1519
1520
1521
1522
1523
1524
1525
1526
1527
1528
1529
1529
1530
1531
1532
1533
1534
1535
1536
1537
1538
1539
1539
1540
1541
1542
1543
1544
1545
1546
1547
1548
1549
1549
1550
1551
1552
1553
1554
1555
1556
1557
1558
1559
1559
1560
1561
1562
1563
1564
1565
1566
1567
1568
1569
1569
1570
1571
1572
1573
1574
1575
1576
1577
1578
1579
1579
1580
1581
1582
1583
1584
1585
1586
1587
1588
1589
1589
1590
1591
1592
1593
1594
1595
1596
1597
1598
1599
1599
1600
1601
1602
1603
1604
1605
1606
1607
1608
1609
1609
1610
1611
1612
1613
1614
1615
1616
1617
1618
1619
1619
1620
1621
1622
1623
1624
1625
1626
1627
1628
1629
1629
1630
1631
1632
1633
1634
1635
1636
1637
1638
1639
1639
1640
1641
1642
1643
1644
1645
1646
1647
1648
1649
1649
1650
1651
1652
1653
1654
1655
1656
1657
1658
1659
1659
1660
1661
1662
1663
1664
1665
1666
1667
1668
1669
1669
1670
1671
1672
1673
1674
1675
1676
1677
1678
1679
1679
1680
1681
1682
1683
1684
1685
1686
1687
1688
1689
1689
1690
1691
1692
1693
1694
1695
1696
1697
1698
1699
1699
1700
1701
1702
1703
1704
1705
1706
1707
1708
1709
1709
1710
1711
1712
1713
1714
1715
1716
1717
171

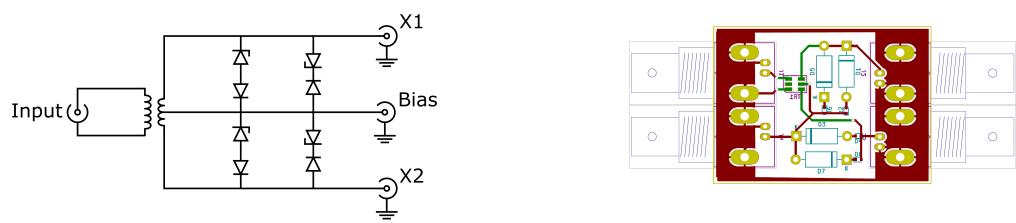

(a) Schematic of center tapped transformer connections

(b) PCB-Layout for center tapped transformer

Figure 7.6

8 Beam Characterization

8.1 Aluminum foil

In fig. 8.1 the inside of the 6-way cross of the first iteration is shown. On one side of the phosphor screen, aluminum foil was attached to simulate the aquadag coating inside the cut CRT. The beam was deflected on the aluminum foil and the BNC output was connected to ground through an ammeter to measure the beam current. As shown in fig. 8.2 there is close to no difference in the filament voltage (and therefore heating power) between an opened and sealed CRT while the beam current on the aluminum foil varies widely. One possible reason could be that electrons scatter. Therefore, a Faraday cup (see section 8.2) was used in the second iteration.

In fig. 8.1 the inside of the 6-way cross of the first iteration is shown. On one side of the phosphor screen, aluminum foil was attached to simulate the aquadag coating inside the cut CRT. The beam was deflected on the aluminum foil and the BNC output was connected to ground through an ammeter to measure the beam current. As shown in fig. 8.2 there is close to no difference in the filament voltage (and therefore heating power) between an opened and sealed CRT while the beam current on the aluminum foil varies widely. One possible reason could be that electrons scatter . Therefore, a Faraday cup (see section 8.2) was used in the second iteration.

1

2

3

4

5

6

7

8

9

10

11

12

13

14

15

16

1 skip: around
18 not all choose
19 the wire path
20 ground

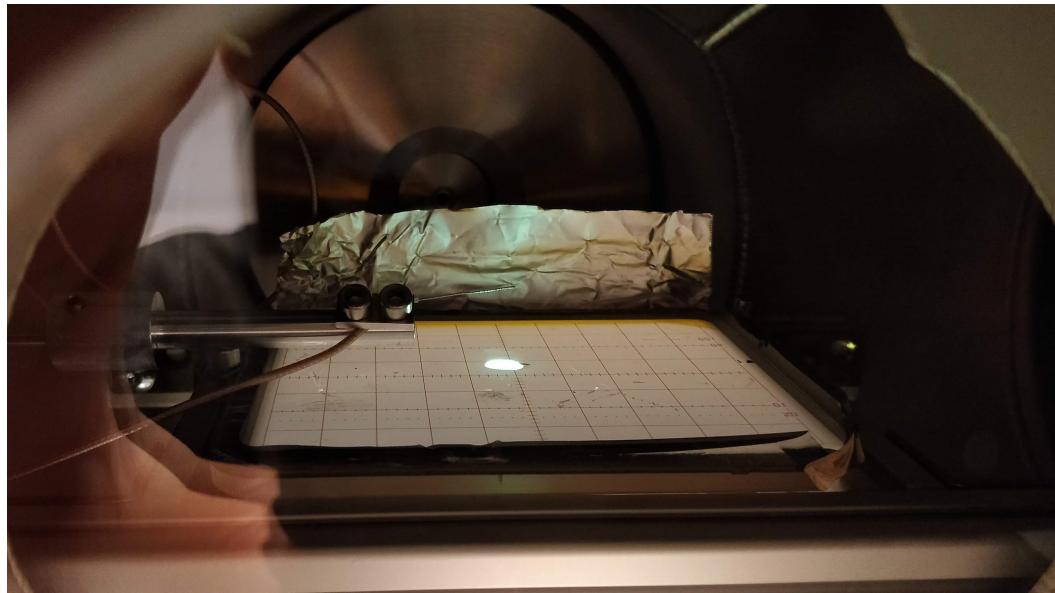


Figure 8.1: Front view of vacuum chamber (first iteration).

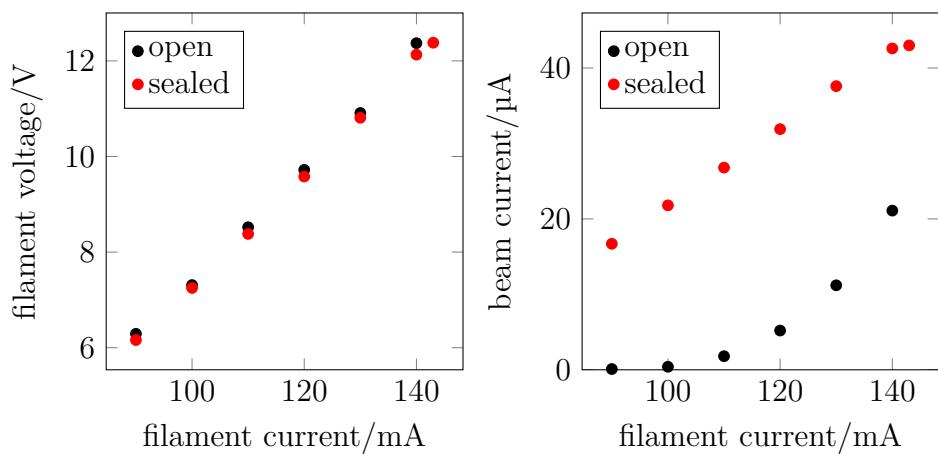


Figure 8.2: Difference in filament voltage and beam current between an open and sealed CRT.

8.2 Faraday cup

In order to accurately measure the full beam current, a Faraday cup was built. A schematic is shown in fig. 8.3. A copper tube was cut at an 45° angle on one side and a Cu-sheet was soldered at the top and bottom. A small hole of around 5 mm was drilled at the top and a coaxial cable was attached on the mantle which connects to a BNC feed through at the top of the chamber. The small opening and angled floor were added, in order to reduce electron loss through back scattering, as indicated by blue arrows in fig. 8.3. At the top surface a phosphor coating was applied, in order to make the beam visible. This made it easier to guide it into the opening hole.

In order to accurately measure the full beam current, a Faraday cup was built. A schematic is shown in fig. 8.3. A copper tube was cut at an 45° angle on one side and a Cu-sheet was soldered at the top and bottom. A small hole of around 5 mm was drilled at the top and a coaxial cable was attached on the mantle which connects to a BNC feed through at the top of the chamber. The small opening and angled floor were added, in order to reduce electron loss through back scattering, as indicated by blue arrows in fig. 8.3. At the top surface a phosphor coating was applied, in order to make the beam visible. This made it easier to guide it into the opening hole.

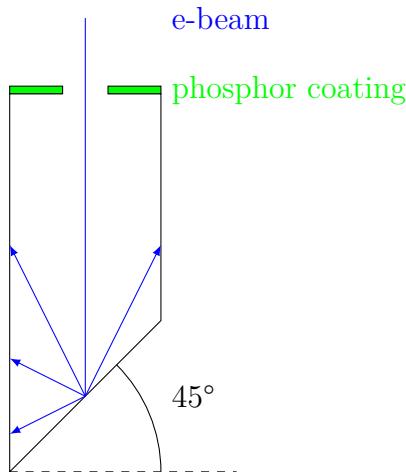


Figure 8.3: Schematics of Faraday cup.

With this improved setup, the beam current was measured again (fig. 8.4). It can be seen, that a current of over $300 \mu\text{A}$ was achieved, which is more than the necessary amount for the experiment. However, through this measurement it became evident that the current is not stable. A measurement on the next day under the same settings resulted in a current between $50 \mu\text{A}$ to $120 \mu\text{A}$.

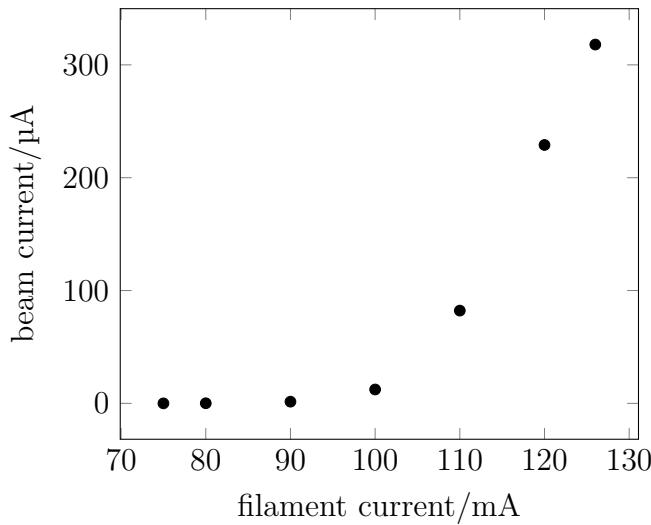


Figure 8.4: Beam current dependence on heater current.

¹ 8.3 Deflection frequency

² This section describes a few observations, that were made when letting the electron
³ beam interact with a short piece of wire, that is mounted to the wobble stick. Originally,
⁴ we hoped to be able to measure the beam waist, using the knife edge method, i.e.
⁵ observing the current transported by the beam, while slowly moving a razor blade
⁶ through the beam path. However the beam is bent, when it passes closely to a
⁷ conductive part. Whenever, we moved our wire close to the beam, the visible spot
⁸ on the Phosphorous screen below was distorted. This will probably complicate the
⁹ measurement of the beam waist in the future. When the wire is connected to an
¹⁰ oscilloscope, one can see a sharp increase in voltage, when it is moved into the beam.
¹¹ This can be used to see whether our deflection plates work properly and to test how
¹² fast we are able to deflect the beam. If the beam oscillates back and forth on a straight
¹³ line and crosses the wire on the midway point, we should see a spike in voltage on the
¹⁴ wire, which repeats with twice the frequency of the beam. If the wire is not on the
¹⁵ midway point, the periods between consecutive spikes should sum up to the period
¹⁶ of the beam's oscillation (see fig. 8.5). At low frequencies we have indeed observed
¹⁷ this behavior. As the frequency is increased, the magnitude of the signal decreases.
¹⁸ This is easily explained by the fact that the remain time close to the wire is inversely
¹⁹ proportional to the frequency and the amplitude of beams deflection. It was possible to
²⁰ see the spikes up to a frequency of 100 kHz, before they where obscured by noise and
²¹ some other periodical, but so far unexplained artifacts. At high deflection frequencies,
²² the wire may also pick up some signal form the capacitive charging and discharging of
²³ the deflection plates and the corresponding oscillating electromagnetic field. In order

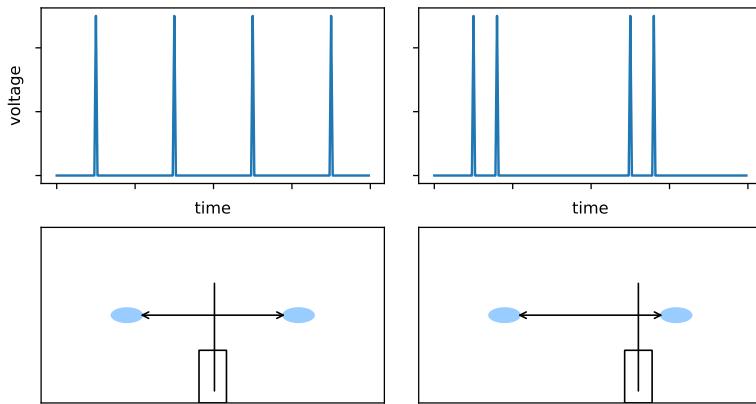


Figure 8.5: Observed Voltage-spikes induced by an electron beam that was deflected periodically across a wire

to be able to see what happens at higher frequencies, a higher beam current and a smaller deflection amplitude would be beneficial. However, the most important factor in order to understand what is happening, is a better focus and a better beam shape.

1
2
3

¹ 9 Next Steps

² To conclude this report, we will point out some of the next steps, that need to be taken
³ in order to advance the electron beam setup.

⁴ **Beam current stability:** The most important challenge at this moment is the ability to
⁵ generate a reproducible, stable, and sufficiently strong beam. In order to achieve
⁶ this, more research on cathodes and their susceptibility to oxygen poisoning needs
⁷ to be conducted. It may also prove useful to add another high voltage power
⁸ supply to the setup, in order to tune the filament potential independently from
⁹ the Wehnelt cylinder.

¹⁰ **Spot size characterisation:** As previously mentioned, our original attempt was, to
¹¹ probe the electron beam's profile using a thin piece of wire on the wobble stick.
¹² However, we have observed that the beam got warped, when passing close to
¹³ conductive materials. Therefore, a different approach is needed.

¹⁴ **Heating mechanism:** As high currents will degrade the filament and cathode, it is
¹⁵ desirable to be able to tune the heater current down to 0 mA continuously. Such
¹⁶ a power supply needs to support a bias voltage of around -2 kV . The current
¹⁷ heater (described in section [4.4](#)) has a minimal current of approximately
¹⁸ 60 mA. It could be improved by using a potentiometer with a larger resistance
¹⁹ range or a variable transformer.

²⁰ **Lissajous Curves:** Regarding the deflection electronics, the first issue that needs to be
²¹ addressed, is the fact that it is not possible to produce a clean sine wave, when
²² a bias voltage is applied to the center tapped transformer. Furthermore, it is
²³ recommended to implement the over voltage protection described previously with
²⁴ very low capacitance diodes. In the future, the setup should be able to produce
²⁵ Lissajous curves at the ^{39}K hyperfine transition frequency of 461.7 MHz.

Todo list

1

■ set date to English	A	2
■ this section is sometimes confusing and already deals with our CRT	2	3
■ you can probably explain it in your own words better -> maybe but I wanted some generally accepted definition (for example this one includes CRTs with multiple electron guns, which I was not aware of)	4	5
■ explain why it has to be a sharp tip already here since it is shown in the picture	2	7
■ "this is a strong statement" -> Yes, too strong of a statement actually	4	8
■ können die Maße stimmen?	4	9
Figure: Image of CRT	6	10
■ mention why it is important -> done	7	11
■ in our ONEnote are some SEM pictures of the cathode	7	12
Figure: Figure of SHV & BNC connector cable.	15	13
Figure: picture of ac bias voltage	17	14
■ check if really 14Ω or if it event exists	17	15
Figure: Image of Stage.	21	16
■ explain more in detail what is the purpose of the chamber, the two iterations are not really important built this chapter rather about the function and operation of the chamber over time due to outgassing the pressure improved)	25	17 18 19
■ water vapor getting into the chamber	25	20
■ explain in connection of the rendering; this makes it easier, if necessary you can get more renderings	25	21 22
■ pure nitrogen name?	25	23
■ Alphagaz TM 1 N_2 purity $\geq 99.999\%$	25	24
■ water vapor getting into the chamber	25	25
■ length=27cm	25	26

1	■ Thyracont exact model is in one note	25
2	■ Thyracont exact model is in one note	26
3	■ orange how many pins and model name? MIL Type C connector	26
4	■ yellow MIL 19 C	26
5	■ orange F: but I'm talking about first iteration	26
6	■ red we also used thin Kapton insulated BNC cable	26
7	■ yellow Viton, maybe also describe the specification of these type of seals	26
8	■ orange rod length? check Solid works	27
9	■ orange rod length? check Solid works	27
10	■ red screwed / with a counter nut	27
11	Figure: Image of CRT mounting mechanism.	27
12	■ red in general make better section titles	27
13	■ red this is not so much of a leak but mainly outgassing / how was the pressure	
14	measured?	27
15	■ orange Optional: insert Foto of CRT's deflection plates - fig:DeflectionSetup	29
16	■ yellow what happens when there is no bias voltage, what is the purpose of it	29
17	■ red to achieve what -> good question! Why did we need that?	29
18	■ orange Find out which amplifier	30
19	■ orange which model?	30
20	■ orange which model?	30
21	■ orange Check amplifier specifications	30
22	■ orange Optional: Go to the lab and measure their performance with an Oszi.	31
23	■ orange Insert fotos of finished circuits in housings	32
24	■ red picture placement and caption is missing -> Done	32
25	■ red skip: around and not all choose the wire path to ground	34