



## LATITUDE™ Programming System

## Device Follow-up Report

Report Created 24 Jul 2021

Date of Birth N/R N/R N/R  
Device ACCOLADE MRI L310/ 839486

Last Office Interrogation  
N/R  
Implant Date  
N/R

## My Alerts

There are no alerts to display.

## Events Since Last Reset (23 Jul 2021)

24 Jul 2021 02:39 RV Auto

## Battery OK

Approximate time to explant: > 8 years  
Magnet Rate 100 min<sup>-1</sup>

One Year Remaining

Explant



## Leads Data

## Implant

## Previous Session

## Most Recent

N/R N/R N/R

Intrinsic Amplitude	N/R mV	N/R mV	13.3 mV@41 min <sup>-1</sup>
Pace Impedance	N/R Ω	N/R Ω	794 Ω
Pace Threshold	N/R V @ N/R ms	N/R	Auto 0.7 V @ 0.4 ms

POST completed. Test started at 23 Jul 2021 09:42

## Settings

## Tachy Settings


Tachy EGM Storage On  
Detection Rate 160 min<sup>-1</sup>

## Brady Settings


Mode	VVIR	Pacing Output	Auto 1.2 V @ 0.4ms
Lower Rate Limit	55 min <sup>-1</sup>	Sensitivity	AGC 0.6 mV
Maximum Sensor Rate	130 min <sup>-1</sup>	Leads Configuration (Pace/Sense)	Bipolar
Refractory	250 - 250 ms	Rate Adaptive Pacing	On
		Minute Ventilation	Passive
		Accelerometer	

## Trends


### Intrinsic Amplitude



### Pace Impedance




### Pace Threshold



Tachy Counters		Since Last Reset	Device Totals
		23 Jul 2021	
<b>Episode Counters</b>			
Total Episodes		0	0
Tachy Episodes		0	0
Nonsustained Episodes		0	0
Brady Counters		Reset Before Last	Since Last Reset
		N/R day(s)	1 day(s)
		N/R to 23 Jul 2021	23 Jul 2021 to Today
<b>Counters</b>			
% Paced		0	74
<b>Intrinsic Promotion</b>			
Rate Hysteresis			
% Successful		0	0

### Histograms Reset Before Last (N/R)

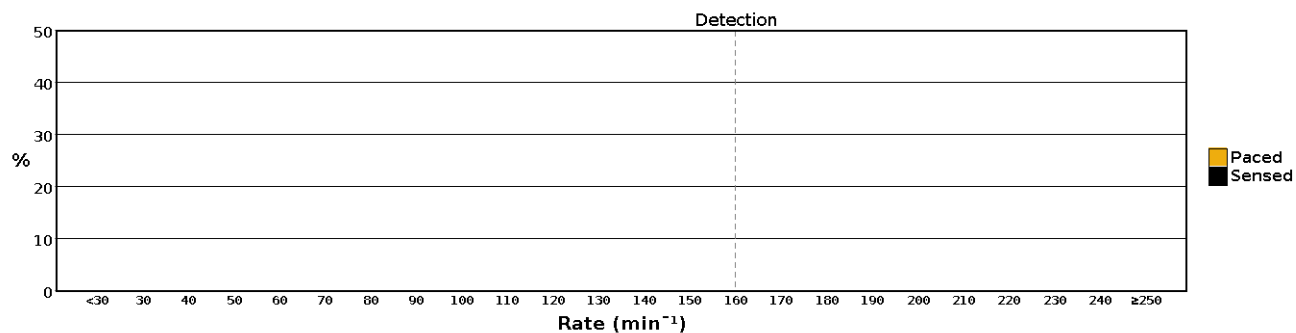

### Histograms Since Last Reset (23 Jul 2021)

