

My Alerts

- 30 Dec 2021 Explant indicator reached
- 14 Feb 2022 10:24 Check Atrial and LV Leads

Events Since Last Reset (03 May 2021)

- 02 Jan 2022 22:31 NonSustV at 177 min⁻¹, Nonsustained
 - 28 Dec 2021 16:10 NonSustV at 153 min⁻¹, Nonsustained
- See last page for full list of Events Since Last Reset.

Battery

- Explant indicator reached on 30 Dec 2021
- Charge Time 15.4 s
- Last Capacitor Re-form 30 Dec 2021 11:42

One Year Remaining

Explant



Leads Data

Implant

12 Mar 2013

Previous Session

Most Recent

Atrial

Intrinsic Amplitude	N/R mV	N/R mV	N/R mV
Pace Impedance	N/R Ω	>2500 Ω	>2500 Ω
Pace Threshold	N/R V @ N/R ms	4.0 V @ 0.4 ms	

Right Ventricular

Intrinsic Amplitude	7.0 mV	8.3 mV	9.5 mV @ 51 min ⁻¹
Pace Impedance	650 Ω	467 Ω	473 Ω
Pace Threshold	0.5 V @ 0.4 ms	0.9 V @ 0.4 ms	

Left Ventricular

Intrinsic Amplitude	12.0 mV	21.2 mV	19.9 mV
Pace Impedance	650 Ω	584 Ω	592 Ω
Pace Threshold	1.3 V @ 0.4 ms	2.0 V @ 0.4 ms	

Shock Vector

Shock Impedance	45 Ω	55 Ω	55 Ω
-----------------	------	------	------

Settings

Ventricular Tachy Settings

VF 230 min ⁻¹ ATP	31J, 41J, 41Jx6
VT 205 min ⁻¹ Scan Ramp	31J, 41J, 41Jx4
VT-1 160 min ⁻¹ Scan Ramp	41J, 41J, 41Jx3


Brady/CRT Settings

Mode	VVIR	Pacing Output	
Lower Rate Limit	65 min ⁻¹	Right Ventricular	2.5 V @ 0.4 ms
Maximum Sensor Rate	130 min ⁻¹	Left Ventricular	3.5 V @ 0.4 ms
RV-Refractory (RVRP)	230 - 250 ms	Sensitivity	
LV-Refractory (LVRP)	250 ms	Atrial	AGC 0.25 mV
Ventricular Pacing Chamber	BiV	Right Ventricular	AGC 0.6 mV
LV Offset	0 ms	Left Ventricular	AGC 1.0 mV
		Leads Configuration (Pace/Sense)	
		Atrial	Bipolar/Off
		Right Ventricular	Bipolar
		Left Ventricular	LVring>>RV / LVtip>>LVring
		Sensors	
		Accelerometer	On

Rhythm ID Update


Last Successful Completion N/R

Trends

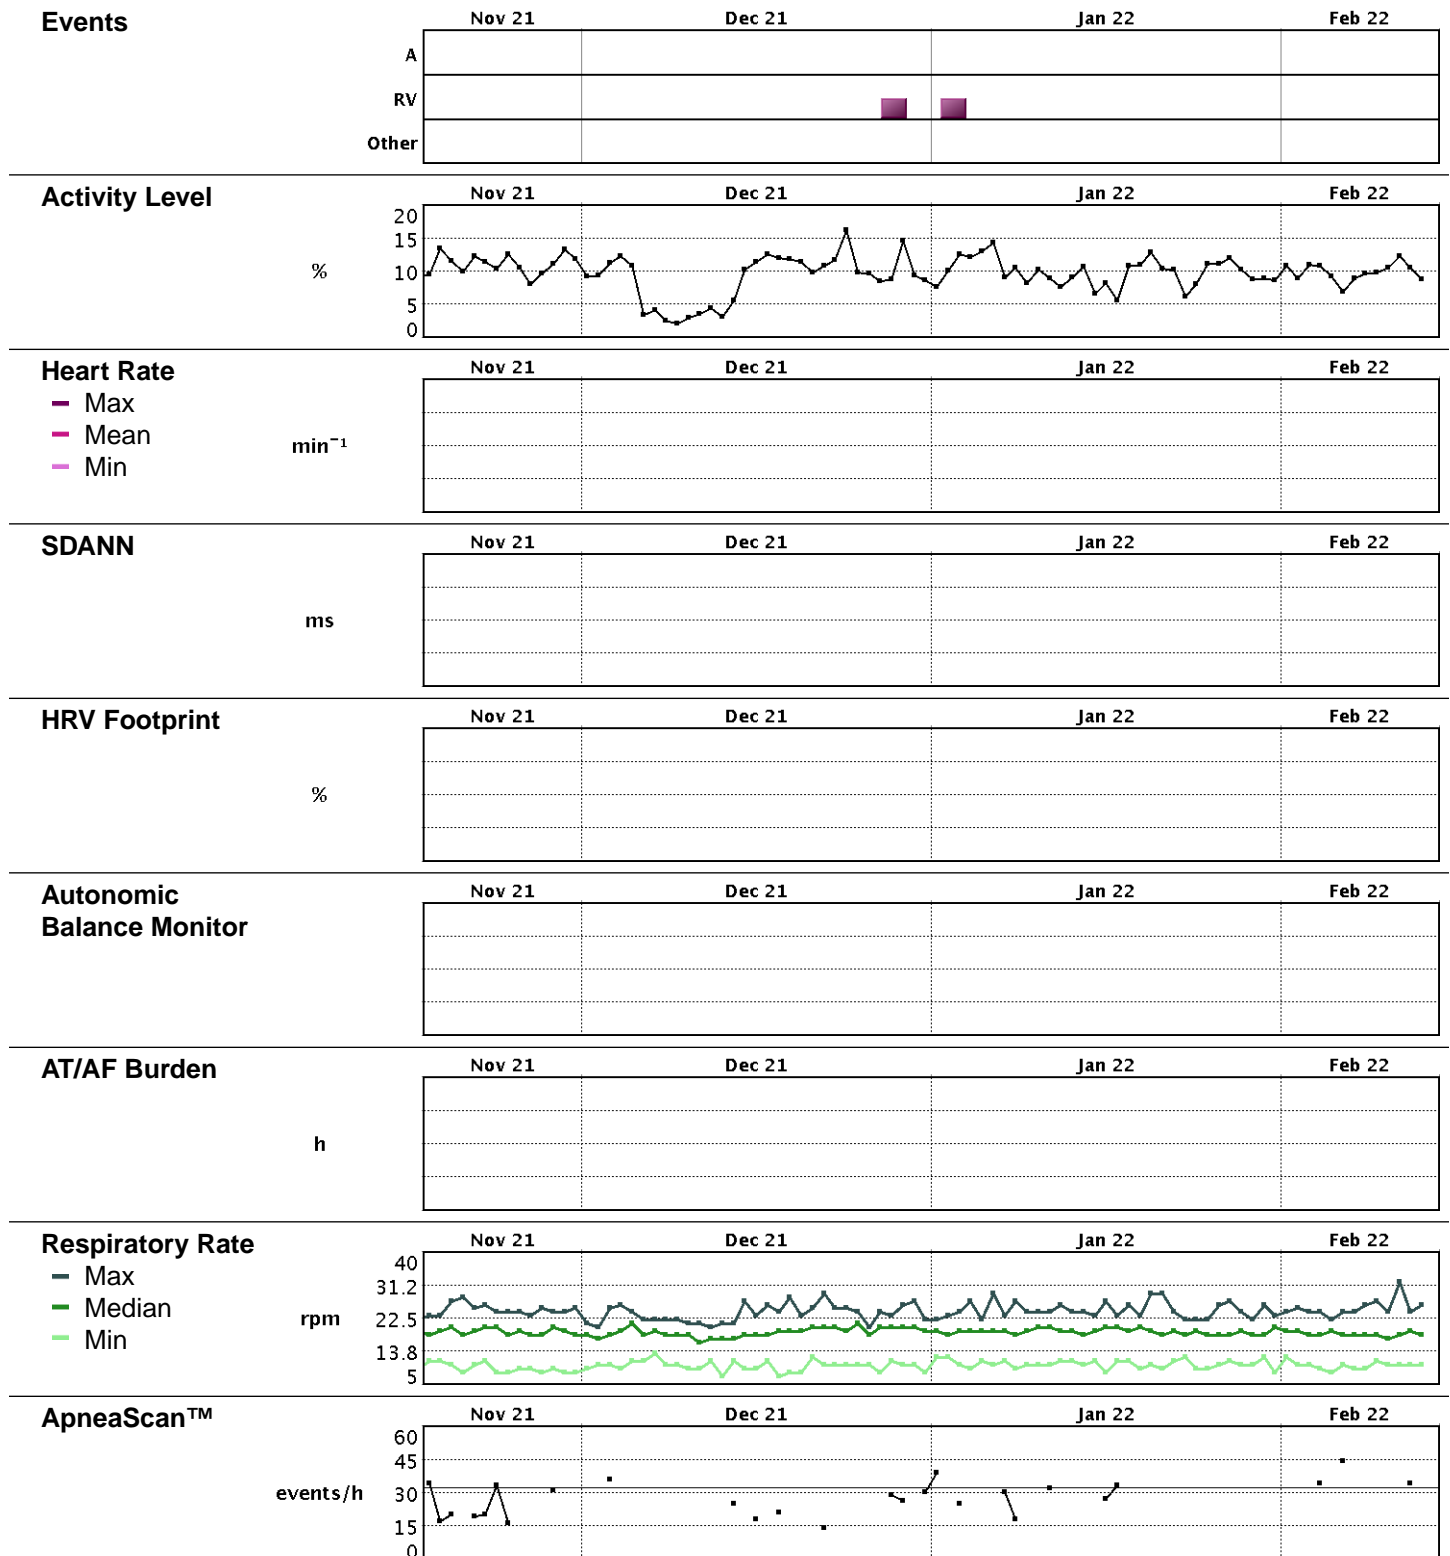


Trends (Continued)


P-Wave Amplitude

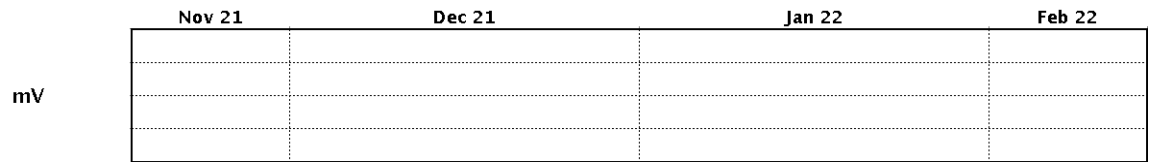


A Pace Impedance

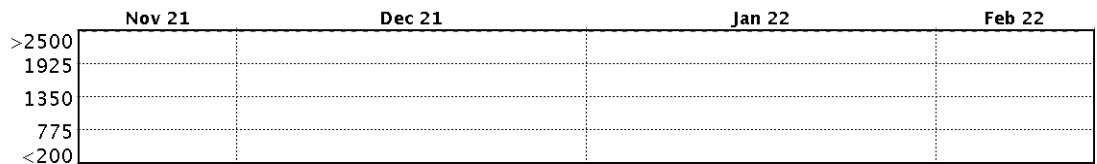


R-Wave (RV) Amplitude

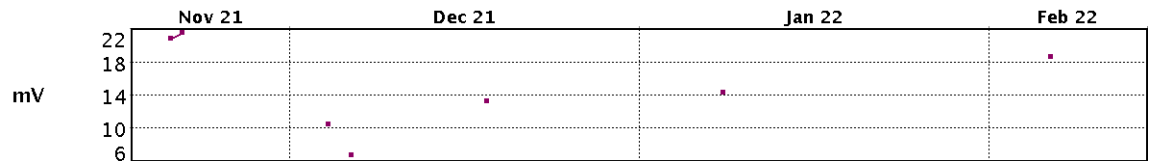


RV Pace Impedance

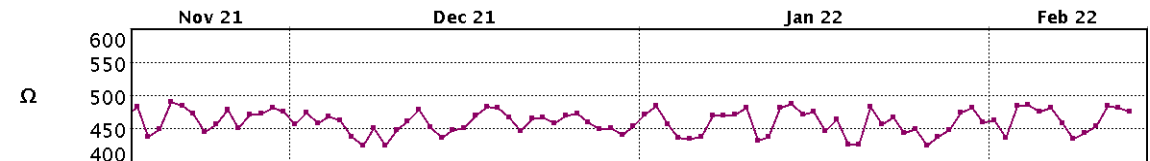


R-Wave (LV) Amplitude

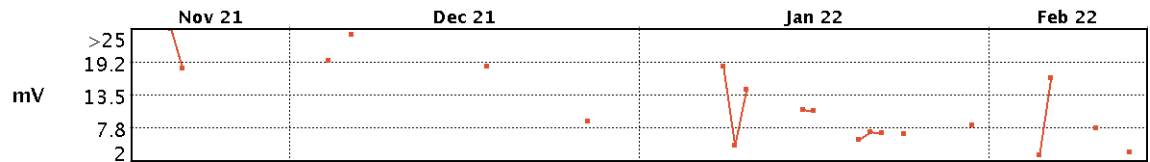

LV Pace Impedance

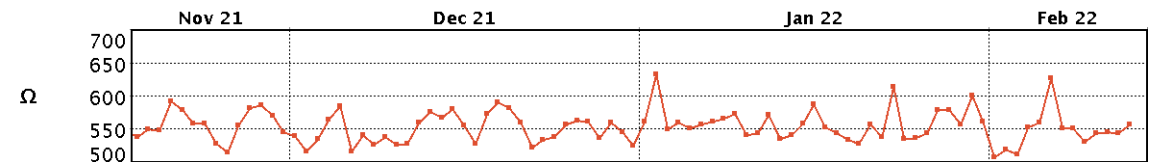


Shock Impedance

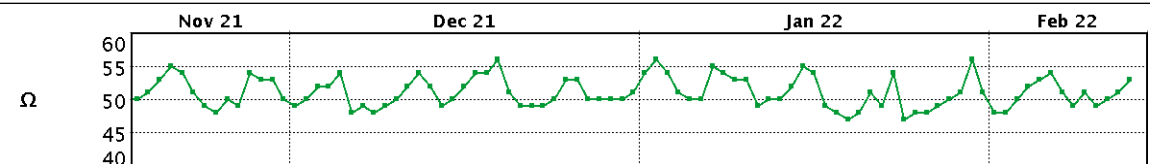


Ventricular Tachy Counters		Since Last Reset	Device Totals
		03 May 2021	
Ventricular Episode Counters			
Total Episodes		8	7.2K
Treated			
VF Therapy		0	0
VT Therapy		0	4
VT-1 Therapy		0	17
Commanded Therapy		0	0
Non-Treated			
No Therapy Programmed		0	0
Nonsustained Episodes		8	7.2K
Other Untreated Episodes		0	7
Ventricular Therapy Counters			
ATP Delivered		0	29
ATP % Successful		0	67
Shocks Delivered		0	6
First Shock % Successful		0	100
Shocks Diverted		0	2
Brady/CRT Counters		Reset Before Last	Since Last Reset
		328 day(s)	287 day(s)
		08 Jun 2020 to 03 May 2021	03 May 2021 to Today
Counters			
% A Paced		100	0
% RV Paced		94	93
% LV Paced		100	100
Intrinsic Promotion			
Rate Hysteresis			
% Successful		0	0
Atrial Arrhythmia			
% AT/AF		0	0
(One Year of Data)			
Total Time in AT/AF (min)		0.0	0.0
(One Year of Data)			
Episodes by Duration			
< 1 minute		0	0
1 min - < 1 hr		0	0
1 hr - < 24 hr		0	0
24 hr - < 48 hr		0	0
> 48 hr		0	0
Total PACs		0	0
Ventricular Counters			
Total PVCs		0	0
Three or More PVCs		0	0

Histograms Reset Before Last (08 Jun 2020)

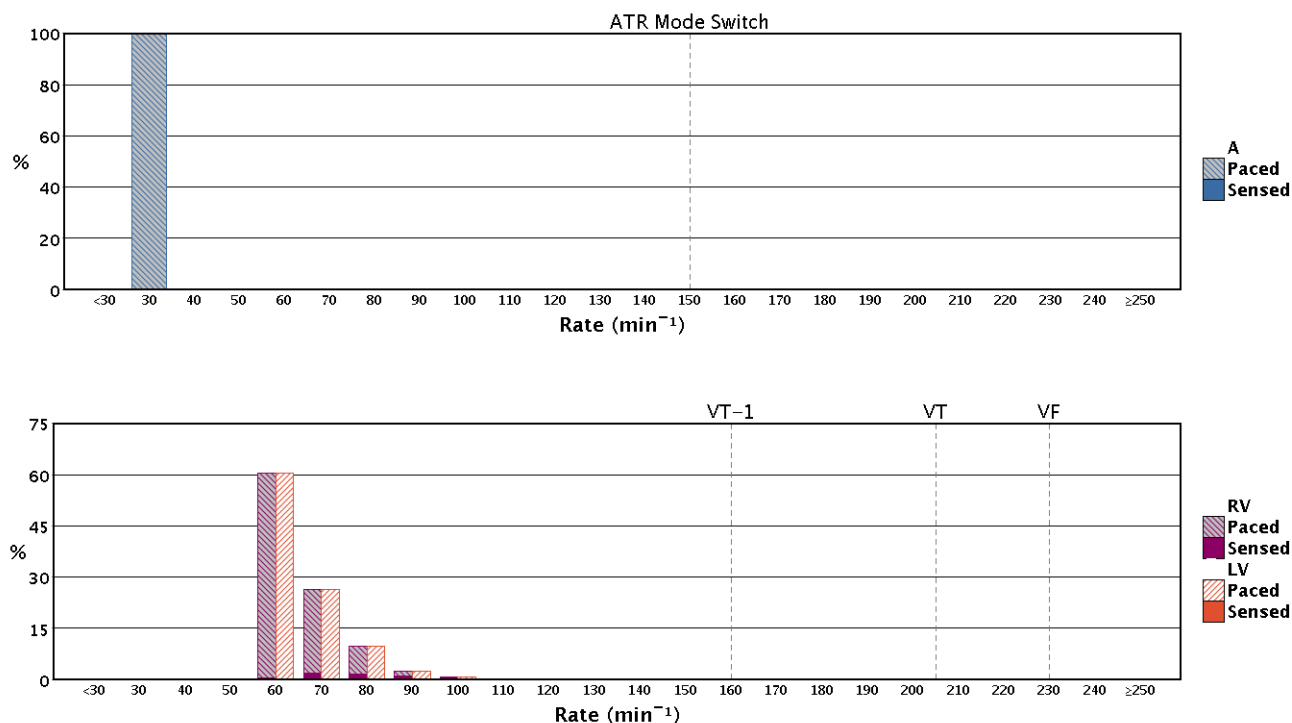

Histograms Since Last Reset (03 May 2021)

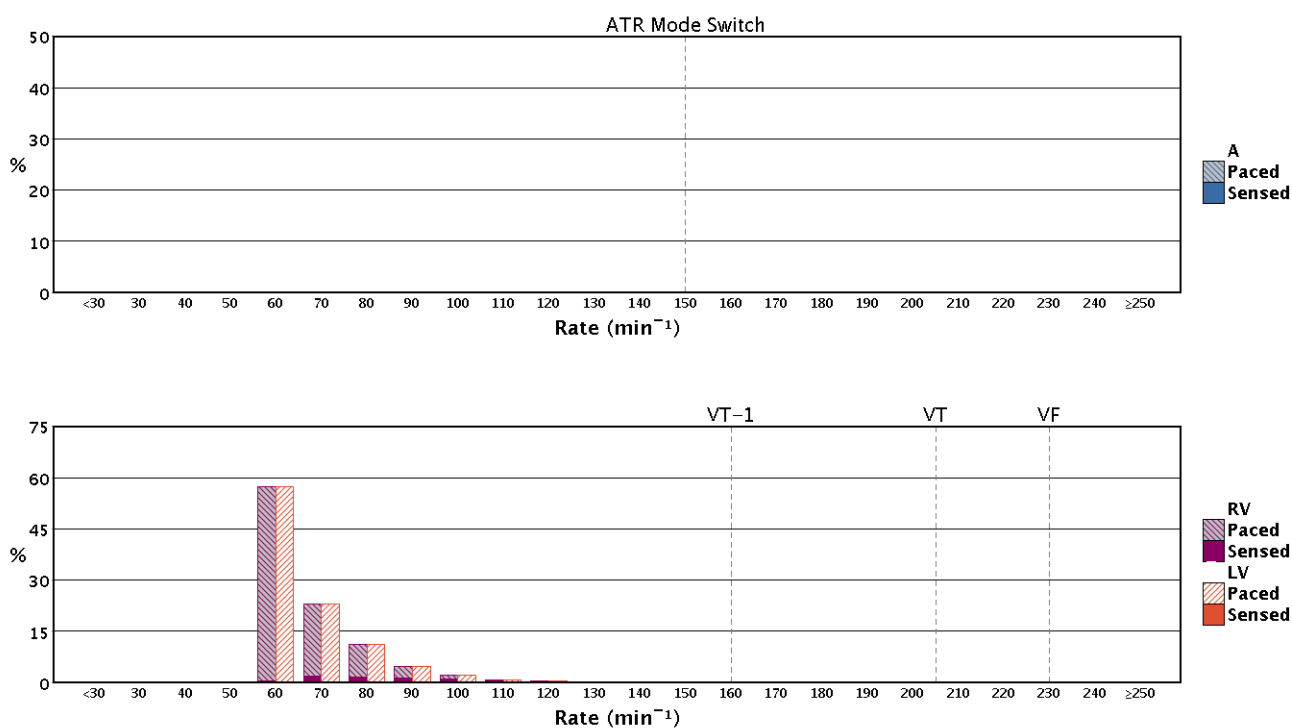

Heart Rate Variability

Last Measured:

Last Measured Data unavailable

Reference:

Reference Data Unavailable

All Events Since Last Reset (03 May 2021)

02 Jan 2022 22:31	NonSustV at 177 min ⁻¹ , Nonsustained
28 Dec 2021 16:10	NonSustV at 153 min ⁻¹ , Nonsustained
29 Oct 2021 22:04	NonSustV at 130 min ⁻¹ , Nonsustained
28 Oct 2021 04:36	NonSustV at 153 min ⁻¹ , Nonsustained
18 Sep 2021 02:11	NonSustV at 159 min ⁻¹ , Nonsustained
16 Sep 2021 09:25	NonSustV at 163 min ⁻¹ , Nonsustained
16 Jul 2021 12:09	NonSustV at 175 min ⁻¹ , Nonsustained
12 Jun 2021 16:37	NonSustV at 127 min ⁻¹ , Nonsustained