

**ZOOM** ® View™ Report Created 12 Nov 2018

**Combined Follow-up Report HOVADÍK 510404, Bronislav** 

Date of Birth 4 Apr 1951

CHARISMA EL ICD D332/243151 Device Monitor + Therapy Tachy Mode

Last Office Interrogation 08 Nov 2018 Implant Date

8 Nov 2018

My Alerts

There are no alerts to display.

**Events Since Last Reset (08 Nov 2018)** 

There are no events to display.

**Battery** OK

Approximate time to explant: > 12 years Charge Time N/R s

Last Capacitor Re-form N/R **One Year Remaining Explant** 

0.7 V @ 0.4 ms

**Leads Data Implant Previous Session Most Recent** 8 Nov 2018 Ventricular Intrinsic Amplitude N/R mV 4.9 mV 5.6 mV @ 75 min<sup>-1</sup> 505 Ω 459 Ω

Pace Impedance  $N/R \Omega$ Pace Threshold N/R V @ N/R ms 0.6 V @ 0.4 ms **Shock Vector** 

Shock Impedance N/R  $\Omega$ 46 Ω 48 Ω

**Settings** 

Ventricular Tachy Settings

VF 220 min<sup>-1</sup> ATP 36J, 41J, 41Jx6 VT 170 min<sup>-1</sup> Burst Ramp/Scan 26J, 31J, 41Jx4

VT-1 150 min<sup>-1</sup> Monitor Only

**Brady Settings** 

VVI **Pacing Output** Mode 50 min<sup>-1</sup> Ventricular Lower Rate Limit

V-Refractory (VRP) 250 ms

2.6 V @ 0.4 ms Sensitivity

Ventricular

AGC 0.6 mV Leads Configuration (Pace/Sense)

Ventricular

Bipolar

Rate Adaptive Pacing

Accelerometer **Passive** 

2868 Software Version: 4.06 D332 Firmware Version: H\_v1.00.00

© 2016 Boston Scientific Corporation or its affiliates. All rights reserved. Page 1 of 6

## **Rhythm ID Update** Last Successful Completion 12 Nov 2018 08:38 Trends Today's Activity: Program and Interrogate Jun 2018 Jul 2018 Aug 2018 Sep 2018 Oct 2018 = Counter Reset = Program Ρ = Interrogate I **Events** Other Most recent Daily Value 3 Day Average measurement: 44 Thoracic 42 42 Impedance Ω 40 26 Respiratory Rate **—** Мах 21 Median \_\_ Min 16 70 53 Night Heart Rate 60 $min^{-1}$ 50

2868 Software Version: 4.06 D332 Firmware Version: H\_v1.00.00 © 2016

Boston Scientific Corporation
or its affiliates. All rights reserved.


Page 2 of 6

Trends (Continued)						
Most recent measurement:					→ Daily Valu	e 3 Day Average
Sleep Incline Insufficient degrees		Jun 2018	Jul 2018	Aug 2018	Sep 2018	Oct 2018
Activity Level 1.0	2-1					***************************************
AP Scan N/R events/h	50					
Heart Rate  Max Mean Min  Min  Min	90 - 70					A A
R-Wave (V) Amplitude	8 7 6 5	Jun 2018	Jul 2018	Aug 2018	Sep 2018	Oct 2018

2868 Software Version: 4.06 D332 Firmware Version: H\_v1.00.00 © 2016


Boston Scientific Corporation
or its affiliates. All rights reserved.

Page 3 of 6

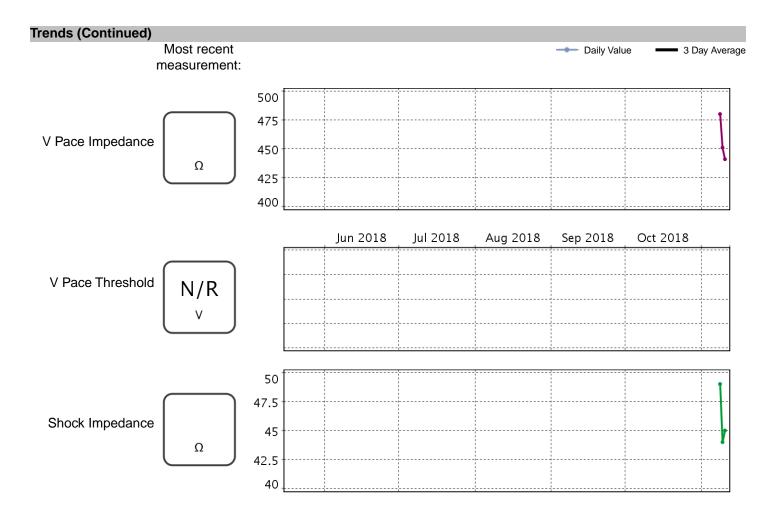


Ventricular Tachy Counters	Since Last Reset 08 Nov 2018	Device Totals
Ventricular Episode Counters		
Total Episodes	0	0
Treated		
VF Therapy	0	0
VT Therapy	0	0
VT-1 Therapy	0	0
Commanded Therapy	0	0
Non-Treated		
No Therapy Programmed	0	0
Nonsustained Episodes	0	0
Other Untreated Episodes	0	0
Ventricular Therapy Counters		
ATP Delivered	0	0
ATP % Successful	0	0
Shocks Delivered	0	0
First Shock % Successful	0	0
Shocks Diverted	0	0
Brady Counters	Reset Before Last	Since Last Reset
	N/R day(s)	4 day(s)
	N/R to 08 Nov 2018	08 Nov 2018 to Today
Counters		
% V Paced	0	<1
Intrinsic Promotion		
Rate Hysteresis		
% Successful	0	0
Clinical Counters	Since Last Reset 08 Nov 2018	Device Totals
MRI Protection Mode	0	0

## **Histograms Reset Before Last (N/R)**

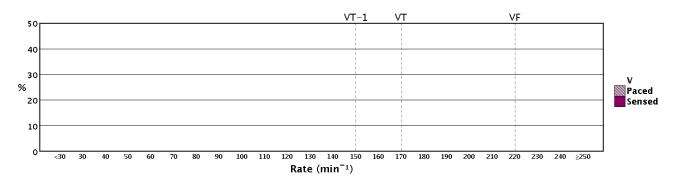

## **Histograms Since Last Reset (08 Nov 2018)**

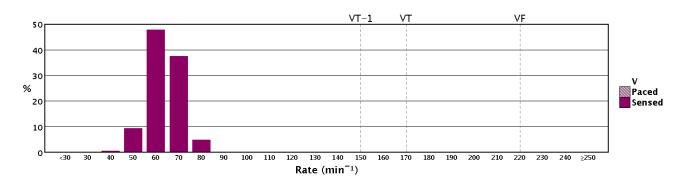

2868 Software Version: 4.06 D332 Firmware Version: H\_v1.00.00 © 2016

Boston Scientific Corporation
or its affiliates. All rights reserved.

Page 6 of 6