

ZOOM ® View[™] Report Created 08 Oct 2018

Combined Follow-up Report ARRAMENDIOVÁ, Jaroslava

Date of Birth N/R N/R N/R

Device AUTOGEN MINI ICD D044/218955 Tachy Mode Monitor + Therapy Last Office Interrogation

05 Oct 2018 Implant Date 5 Oct 2018

My Alerts

There are no alerts to display.

Events Since Last Reset (05 Oct 2018)

05 Oct 2018 09:00 VF at 276 min⁻¹, Induced: 26J

Battery OK

Approximate time to explant: > 5 years
Charge Time N/R s

Last Capacitor Re-form N/R

One Year Remaining Explant

19.3 mV

Leads Data Implant Previous Session Most Recent
5 Oct 2018

Ventricular

N/R mV

Intrinsic Amplitude
Pace Impedance

Pace Impedance N/R Ω Pace Threshold N/R V @ N/R ms Shock Vector

 $/R \Omega$ 389 Ω /R ms 0.4 V @ 0.4 ms

467 Ω Auto 0.5 V @ 0.4 ms

>25.0 mV @ 92 min⁻¹

2.6 V @ 0.4 ms

.4 ms Auto 0.5 V @ 0.4 ms

Shock Impedance N/R Ω 81 Ω 79 Ω

Settings

Ventricular Tachy Settings

VF 220 min⁻¹ ATP 36J, 41J, 41Jx6 VT 170 min⁻¹ Burst Ramp/Scan 31J, 36J, 41Jx4 VT-1 150 min⁻¹ ATP1 Off ATP2 Off 41J, 41J, 41Jx3

Brady Settings

Mode VVI Pac Lower Rate Limit 40 min⁻¹ Ve V-Refractory (VRP) 250 ms Sen

Pacing Output
Ventricular
Sensitivity

Ventricular AGC 0.6 mV

Leads Configuration (Pace/Sense)

Ventricular Bipolar

Rate Adaptive Pacing

Minute Ventilation Passive
Accelerometer Passive

2868 Software Version: 4.04 D044 Firmware Version: E_v1.02.00(2.01)

© 2016

Boston Scientific Corporation
or its affiliates. All rights reserved.

Page 1 of 4

Clinician Signature:


Last Successful Com	pletion	1	08 Oct 20	18 08:39		
Trends						
Events			Jul 18	Aug 18	Sep 18	Oct 18
		v				
		Other				
Activity Level			Jul 18	Aug 18	Sep 18	Oct 18
		2.5 1.9				
	%	1.2				
		0.6				رب.
Heart Rate		0 📖	Jul 18	Aug 18	Sep 18	Oct 18
- Max		120	•			
- Maan	min ⁻¹	90				`
Min		75				
		60				
Respiratory Rate		40	Jul 18	Aug 18	Sep 18	Oct 18
- Max		32.5				
MedianMin	rpm	25				
— IVIIII		17.5				
AP Scan			Jul 18	Aug 18	Sep 18	Oct 18
		60 45				/
e	vents/h	30				
		15				
		0 🖳				
R-Wave (V)		24	Jul 18	Aug 18	Sep 18	Oct 18
Amplitude		23.5				,
	mV	23				/
		22.5				
V Pace Impedance			Jul 18	Aug 18	Sep 18	Oct 18
		500 475				
	Ω	450				
		425				
		400				
V Pace Threshold		_	Jul 18	Aug 18	Sep 18	Oct 18
		ļ				
	V					
Shock Impedance			Jul 18	Aug 18	Sep 18	Oct 18
-		80 77.5				
	Ω	75				•
		72.5				
368 Software Version: 4.04		70		© 2016	Clinician Signature:	
,00 0011Wall Vol31011. 4.04				C =010	Lunician Signature:	

D044 Firmware Version: E_v1.02.00(2.01)


Boston Scientific Corporation or its affiliates. All rights reserved.
Page 2 of 4

Ventricular Tachy Counters	Since Last Reset 05 Oct 2018	Device Totals
Ventricular Episode Counters		
Total Episodes	1	1
Treated		
VF Therapy	1	1
VT Therapy	0	0
VT-1 Therapy	0	0
Commanded Therapy	0	0
Non-Treated		
No Therapy Programmed	0	0
Nonsustained Episodes	0	0
Other Untreated Episodes	0	0
Ventricular Therapy Counters		
ATP Delivered	0	0
ATP % Successful	0	0
Shocks Delivered	1	1
First Shock % Successful	100	100
Shocks Diverted	0	0
Brady Counters	Reset Before Last	Since Last Reset
	N/R day(s)	3 day(s)
	N/R to 05 Oct 2018	05 Oct 2018 to Today
Counters		
% V Paced	0	<1
Intrinsic Promotion		
Rate Hysteresis		
% Successful	0	0
Clinical Counters	Since Last Reset 05 Oct 2018	Device Totals
MRI Protection Mode	0	0

Histograms Reset Before Last (N/R)

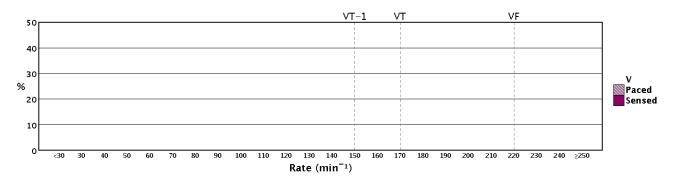

Histograms Since Last Reset (05 Oct 2018)

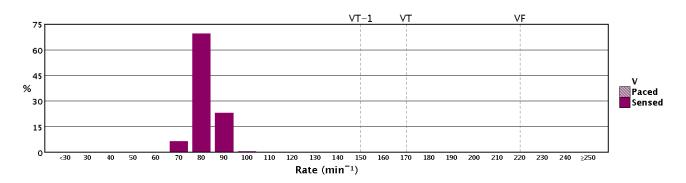

Clinician Signature: