

**LATITUDE™ Programming System**

Report Created 23 Feb 2022

**Device Follow-up Report****Krajca 540702, Miroslav**

Date of Birth N/R N/R N/R

Device CHARISMA CRT-D G324/ 500899

Tachy Mode Monitor + Therapy

Last Office Interrogation

**22 Feb 2022**

Implant Date

**22 Feb 2022****My Alerts**

There are no alerts to display.

**Events Since Last Reset (22 Feb 2022)**

23 Feb 2022 07:27 SAM, Respiratory Sensor Vector Switched

22 Feb 2022 12:30 LV Auto

22 Feb 2022 12:28 RV Auto

**Battery OK**

Approximate time to explant: &gt; 8 years

Charge Time N/R s

Last Capacitor Re-form N/R

One Year Remaining

Explant

**Leads Data****Implant**

22 Feb 2022

**Previous Session****Most Recent****Atrial**

Intrinsic Amplitude N/R mV

Pace Impedance N/R  $\Omega$ 

Pace Threshold N/R V @ N/R ms

0.5 mV

>3000  $\Omega$ 

N/R

N/R mV

>3000  $\Omega$ 

Test Failed

**Right Ventricular**

Intrinsic Amplitude N/R mV

Pace Impedance N/R  $\Omega$ 

Pace Threshold N/R V @ N/R ms

Paced mV

634  $\Omega$ 

Auto 0.8 V @ 0.4 ms

>25.0 mV @ 48 min<sup>-1</sup>669  $\Omega$ 

Auto 0.8 V @ 0.4 ms

**Left Ventricular**

Intrinsic Amplitude N/R mV

Pace Impedance N/R  $\Omega$ 

Pace Threshold N/R V @ N/R ms

Paced mV

654  $\Omega$ 

Auto 2.5 V @ 1.0 ms

4.9 mV

706  $\Omega$ 

Auto 2.2 V @ 1.0 ms

**Shock Vector**Shock Impedance N/R  $\Omega$ 58  $\Omega$ 58  $\Omega$ **Settings****Ventricular Tachy Settings**VF 200 min<sup>-1</sup> ATP 41J, 41J, 41Jx6VT 165 min<sup>-1</sup> Burst Ramp 41J, 41J, 41Jx4**Brady/CRT Settings**

Mode VVIR

Lower Rate Limit 75 min<sup>-1</sup>Maximum Sensor Rate 130 min<sup>-1</sup>

RV-Refractory (RVRP) 230 - 250 ms

LV-Refractory (LVRP) 250 ms

Ventricular Pacing Chamber BiV

LV Offset -20 ms

**Pacing Output**

Right Ventricular

Left Ventricular

**Sensitivity**

Atrial

Right Ventricular

Left Ventricular

**Leads Configuration (Pace/Sense)**

Atrial

Right Ventricular

Left Ventricular

**Rate Adaptive Pacing**

Accelerometer

Auto 2.0 V @ 0.4ms

Auto 3.2 V @ 1.0ms

AGC 0.25 mV

AGC 0.6 mV

AGC 1.0 mV

Bipolar  
Bipolar  
LVtip>>Can / LVtip>>LVring

On

## Rhythm ID Update

Last Successful Completion

N/R

## Trends

Most recent  
measurement:

		Sep 2021	Oct 2021	Nov 2021	Dec 2021	Jan 2022	Feb 2022
P-Wave Amplitude	N/R mV						
A Pace Impedance	N/R $\Omega$						
A Pace Threshold	V						
R-Wave (RV) Amplitude	N/R mV						
RV Pace Impedance	N/R $\Omega$						

## Trends

Most recent  
measurement:

RV Pace Threshold

V

Sep 2021	Oct 2021	Nov 2021	Dec 2021	Jan 2022	Feb 2022

R-Wave (LV) Amplitude

N/R  
mV


LV Pace Impedance

N/R  
Ω


LV Pace Threshold


N/R  
V


Shock Impedance

N/R  
Ω


Ventricular Tachy Counters		Since Last Reset 22 Feb 2022	Device Totals
<b>Ventricular Episode Counters</b>			
Total Episodes		0	0
Treated			
VF Therapy		0	0
VT Therapy		0	0
VT-1 Therapy		0	0
Commanded Therapy		0	0
Non-Treated			
No Therapy Programmed		0	0
Nonsustained Episodes		0	0
Other Untreated Episodes		0	0
<b>Ventricular Therapy Counters</b>			
ATP Delivered		0	0
ATP % Successful		0	0
Shocks Delivered		0	0
First Shock % Successful		0	0
Shocks Diverted		0	0
Brady/CRT Counters		Reset Before Last 0 day(s) 22 Feb 2022 to 22 Feb 2022	Since Last Reset 0 day(s) 22 Feb 2022 to Today
<b>Counters</b>			
% A Paced		70	0
% RV Paced		97	100
% LV Paced		93	100
<b>Intrinsic Promotion</b>			
Rate Hysteresis			
% Successful		0	0
<b>Atrial Arrhythmia</b>			
% AT/AF		N/R	N/R
Total Time in AT/AF		N/R	N/R
Episodes by Duration			
< 1 minute		0	0
1 min - < 1 hr		0	0
1 hr - < 24 hr		0	0
24 hr - < 48 hr		0	0
> 48 hr		0	0
Total PACs		0	0
<b>Ventricular Counters</b>			
Total PVCs		0	0
Three or More PVCs		0	0
Clinical Counters		Since Last Reset 22 Feb 2022	Device Totals
MRI Protection Mode		0	0

### Histograms Reset Before Last (22 Feb 2022)

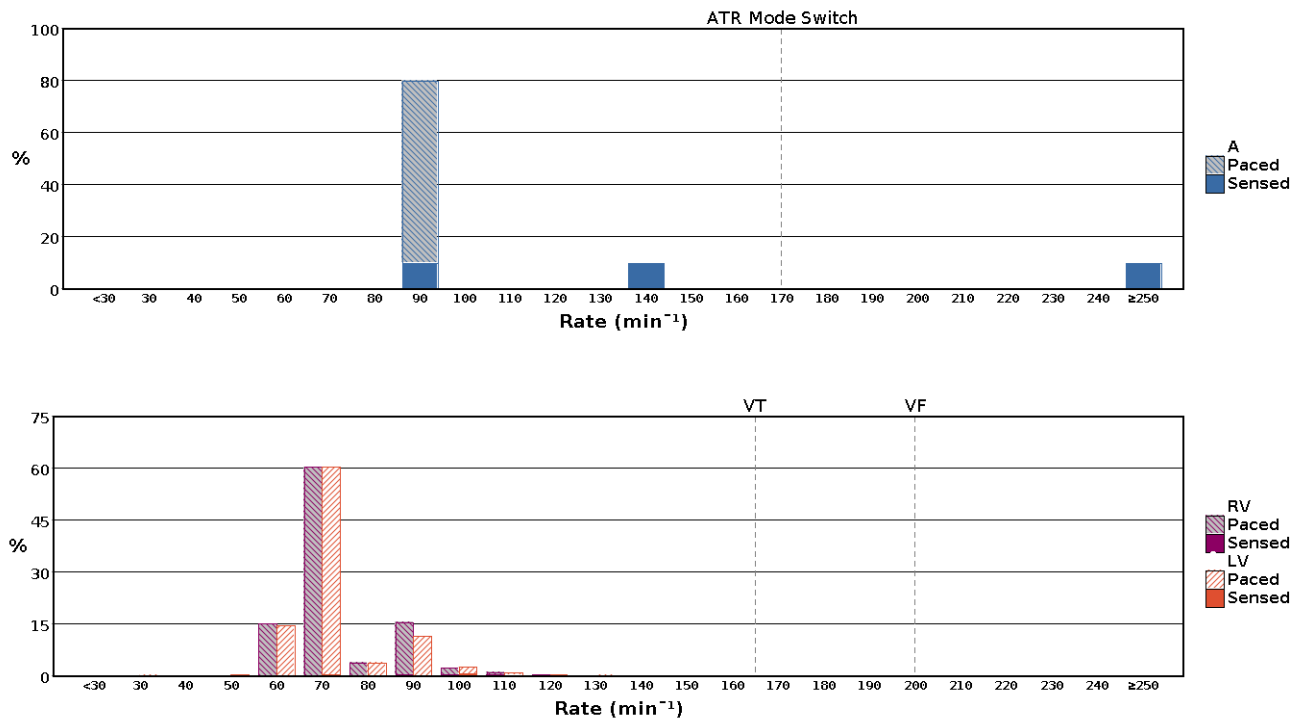

### Histograms Since Last Reset (22 Feb 2022)

