



ZOOM® View™

Combined Follow-up Report

Hucik, Stepán

Date of Birth 7 Jan 1944
Device INCEPTA CRT-D P162/119874
Tachy Mode Monitor + Therapy

Report Created 08 Jun 2020

Last Office Interrogation

10 Jun 2019

Implant Date

12 Mar 2013

My Alerts

⚠ 08 Jun 2020 10:28 Check Atrial and LV Leads

Events Since Last Reset (04 Jun 2018)

26 May 2020 10:22 NonSustV at 163 min⁻¹, Nonsustained29 Apr 2020 05:28 NonSustV at 155 min⁻¹, Nonsustained

See last page for full list of Events Since Last Reset.

Battery OK

Approximate time to explant: 1.5 years

Charge Time 12.1 s

Last Capacitor Re-form 28 Apr 2020 08:35

One Year Remaining

Explant



Leads Data

Implant

12 Mar 2013

Previous Session

Most Recent

Atrial

Intrinsic Amplitude N/R mV N/R mV N/R mV

Pace Impedance N/R Ω <200 Ω >2500 Ω

Pace Threshold N/R V @ N/R ms 4.0 V @ 0.4 ms

Right Ventricular

Intrinsic Amplitude 7.0 mV 6.3 mV 8.6 mV @ 39 min⁻¹

Pace Impedance 650 Ω 495 Ω 462 Ω

Pace Threshold 0.5 V @ 0.4 ms 1.1 V @ 0.4 ms 0.7 V @ 0.4 ms

Left Ventricular

Intrinsic Amplitude 12.0 mV >25.0 mV 22.0 mV

Pace Impedance 650 Ω 494 Ω 543 Ω

Pace Threshold 1.3 V @ 0.4 ms 1.2 V @ 0.4 ms 1.7 V @ 0.4 ms

Shock Vector

Shock Impedance 45 Ω 52 Ω 52 Ω

Settings

Ventricular Tachy Settings

VF 230 min⁻¹ ATP 31J, 41J, 41Jx6VT 205 min⁻¹ Scan Ramp 31J, 41J, 41Jx4VT-1 160 min⁻¹ Scan Ramp 41J, 41J, 41Jx3

Brady/CRT Settings

Mode VVIR

Lower Rate Limit 65 min⁻¹Maximum Sensor Rate 130 min⁻¹

RV-Refractory (RVRP) 230 - 250 ms

LV-Refractory (LVRP) 250 ms

Ventricular Pacing Chamber BiV

LV Offset 0 ms

Pacing Output

Right Ventricular 2.5 V @ 0.4 ms

Left Ventricular 3.0 V @ 0.4 ms

Sensitivity

Atrial AGC 0.25 mV

Right Ventricular AGC 0.6 mV

Left Ventricular AGC 1.0 mV

Leads Configuration (Pace/Sense)

Atrial Bipolar/Off

Right Ventricular Bipolar

Left Ventricular LVring>>RV / LVtip>>LVring


Sensors

Accelerometer On

Rhythm ID Update


Last Successful Completion N/R

Trends

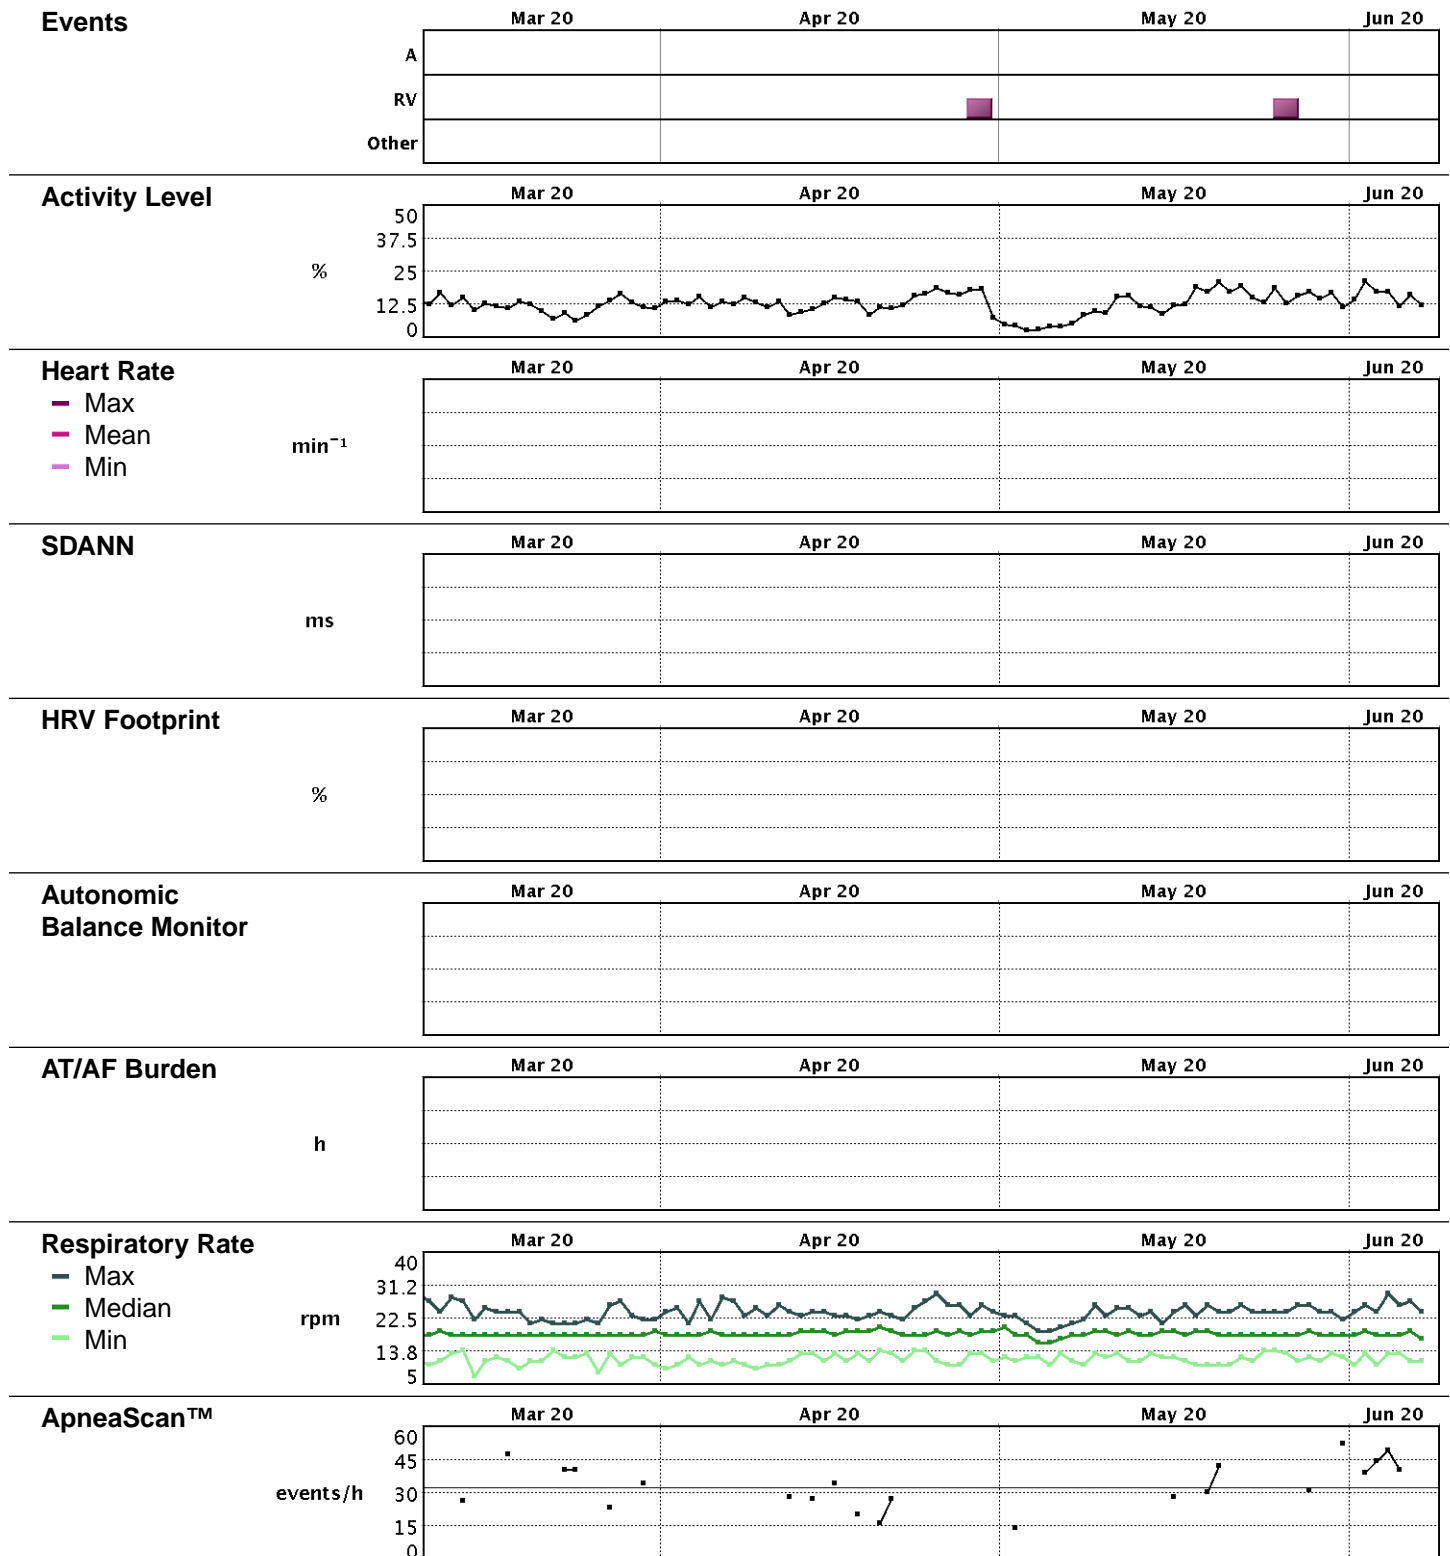


Trends (Continued)


P-Wave Amplitude

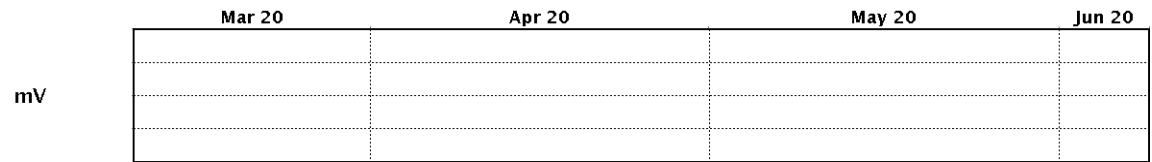


A Pace Impedance

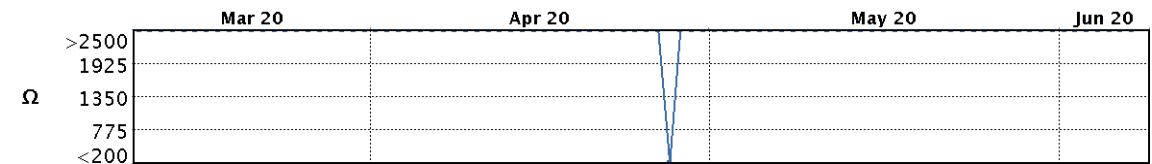


R-Wave (RV) Amplitude

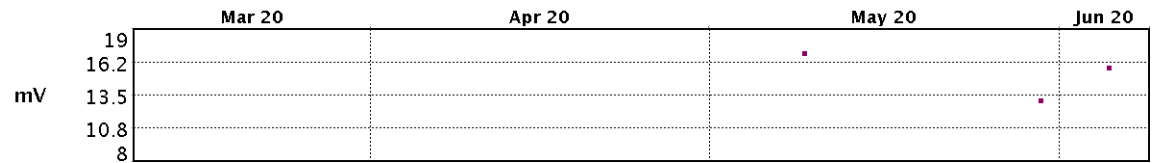


RV Pace Impedance

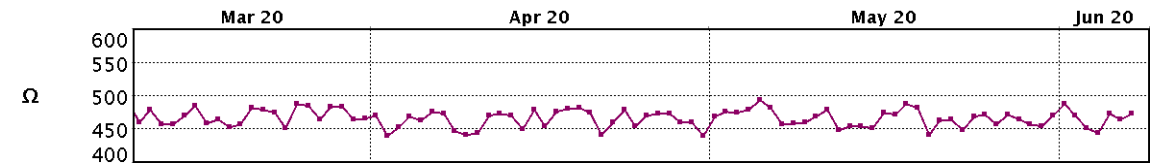


R-Wave (LV) Amplitude

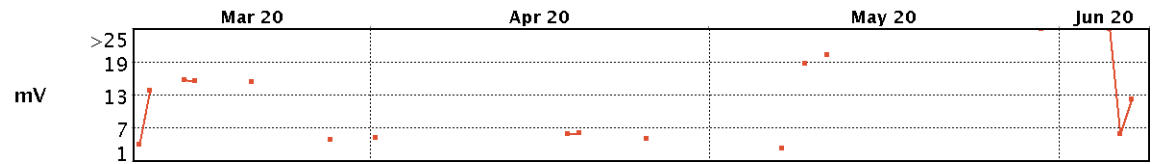

LV Pace Impedance

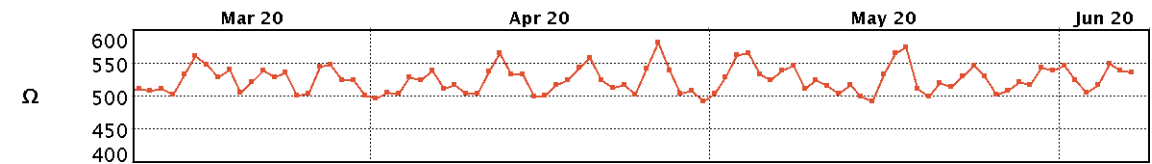


Shock Impedance

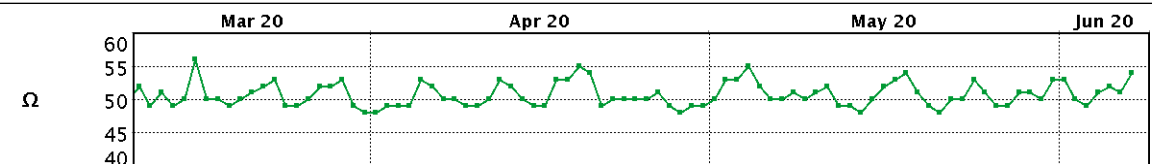


Ventricular Tachy Counters	Since Last Reset 04 Jun 2018	Device Totals
Ventricular Episode Counters		
Total Episodes	13	7.2K
Treated		
VF Therapy	0	0
VT Therapy	0	4
VT-1 Therapy	0	17
Commanded Therapy	0	0
Non-Treated		
No Therapy Programmed	0	0
Nonsustained Episodes	13	7.2K
Other Untreated Episodes	0	7
Ventricular Therapy Counters		
ATP Delivered	0	29
ATP % Successful	0	67
Shocks Delivered	0	6
First Shock % Successful	0	100
Shocks Diverted	0	2
Brady/CRT Counters	Reset Before Last 1907 day(s) 14 Mar 2013 to 04 Jun 2018	Since Last Reset 735 day(s) 04 Jun 2018 to Today
Counters		
% A Paced	0	0
% RV Paced	90	94
% LV Paced	97	100
Intrinsic Promotion		
Rate Hysteresis		
% Successful	0	0
Atrial Arrhythmia		
% AT/AF	N/R	0
(One Year of Data)		
Total Time in AT/AF (min)	N/R	0.0
(One Year of Data)		
Episodes by Duration		
< 1 minute	0	0
1 min - < 1 hr	0	0
1 hr - < 24 hr	0	0
24 hr - < 48 hr	0	0
> 48 hr	0	0
Total PACs	0	0
Ventricular Counters		
Total PVCs	97	0
Three or More PVCs	9	0

Histograms Reset Before Last (14 Mar 2013)

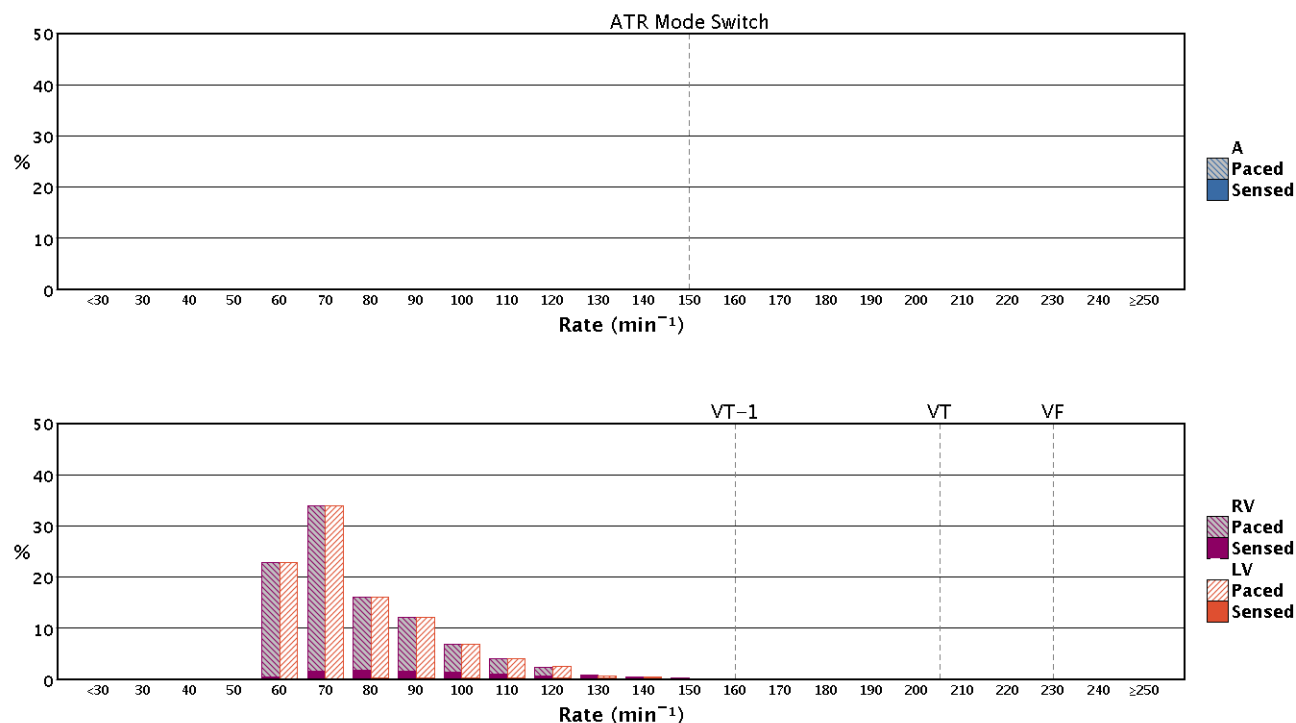

Histograms Since Last Reset (04 Jun 2018)

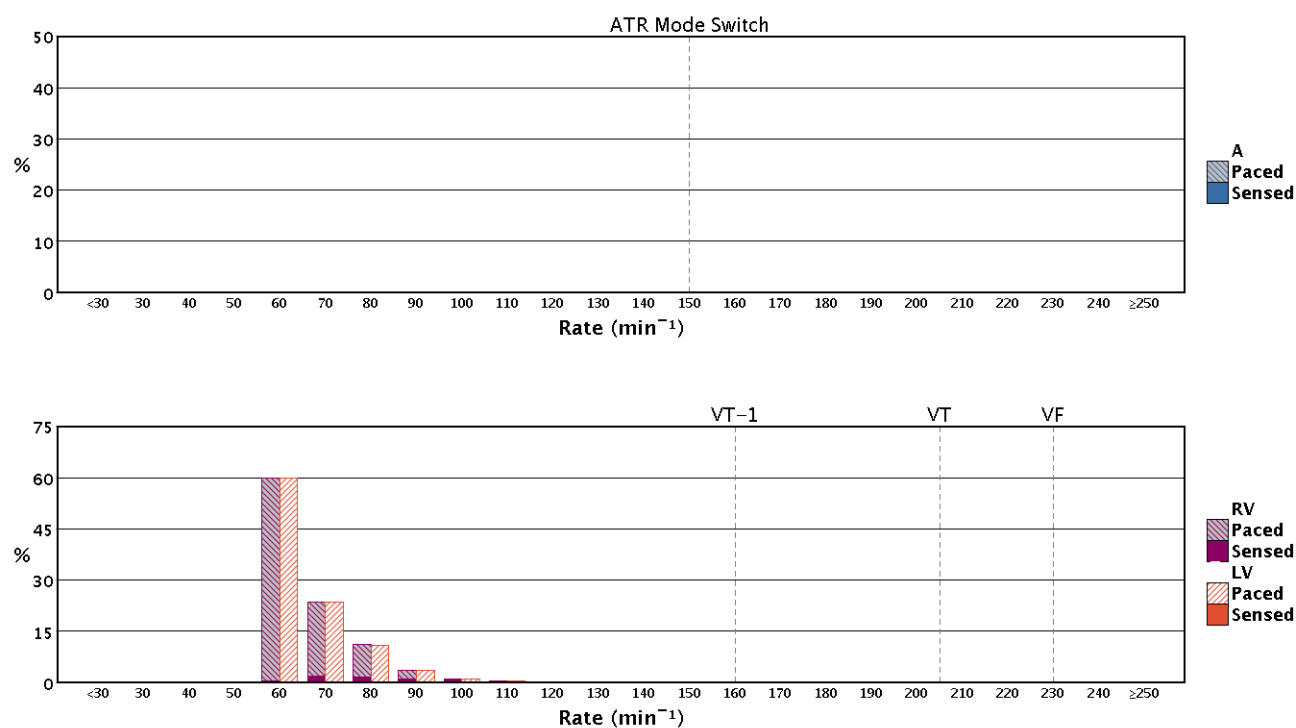

Heart Rate Variability

Last Measured:

Last Measured Data unavailable

Reference:

Reference Data Unavailable

All Events Since Last Reset (04 Jun 2018)

26 May 2020 10:22	NonSustV at 163 min ⁻¹ , Nonsustained
29 Apr 2020 05:28	NonSustV at 155 min ⁻¹ , Nonsustained
31 Aug 2019 06:49	NonSustV at 166 min ⁻¹ , Nonsustained
27 Jul 2019 01:11	NonSustV at 165 min ⁻¹ , Nonsustained
07 Mar 2019 21:06	NonSustV at 159 min ⁻¹ , Nonsustained
30 Nov 2018 10:37	NonSustV at 136 min ⁻¹ , Nonsustained
05 Nov 2018 13:35	NonSustV at 143 min ⁻¹ , Nonsustained
25 Oct 2018 00:58	NonSustV at 128 min ⁻¹ , Nonsustained
02 Sep 2018 05:41	NonSustV at 163 min ⁻¹ , Nonsustained
03 Aug 2018 22:41	NonSustV at 145 min ⁻¹ , Nonsustained