

	ZOOM ® View™		Report Created 08 Nov 2016
	Selected Episodes Report		
	KRÍZ, Karel		Last Office Interrogation
	Date of Birth	30 Aug 1954	31 Aug 2016
	Device	AUTOGEN X4 CRT-D G179/136339	Implant Date
	Tachy Mode	Monitor + Therapy	12 Oct 2015

Event V-49: 01 Sep 2016 17:32

**VF Event Onset** Avg A Rate: 62 min<sup>-1</sup> Avg V Rate: 364 min<sup>-1</sup> Detection: Rhythm ID

Template: 27 Jul 2016 12:12 RhythmMatch™ Threshold: 94 %

At V-Detect

Avg A Rate: 63 min<sup>-1</sup> Avg V Rate: 337 min<sup>-1</sup>

Rate Zone: VF

Stability: (92 ms, Off) V>A Rate: (True, Off) AFib: (False, Off)

RhythmID Correlated: False RhythmMatch™: 0 % SRD Met: (False, Off) ATP Timeout: False

Attempt 1, 36 J V Shock Elapsed Time: 00:00:10 **Shock Information:** Charge Time: 0.9 s Lead Impedance: 53  $\Omega$ Lead Polarity: Initial


## **Event Ended 00:00:44**





2868 Software Version: 3.07 G179 Firmware Version: E\_v1.02.00(2.01)


© 2014 Boston Scientific Corporation or its affiliates. All rights reserved. Page 1 of 4

Clinician Signature:

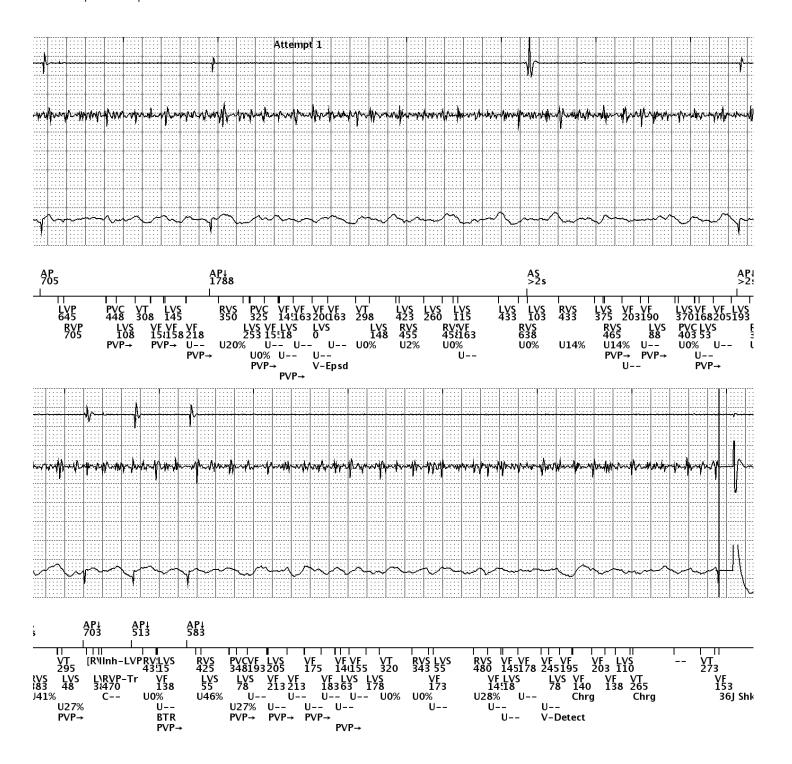

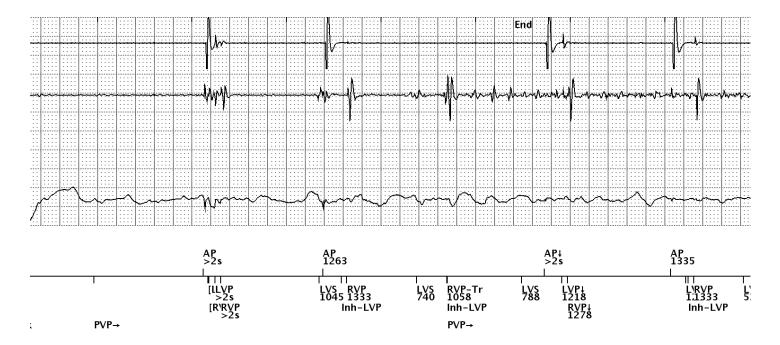

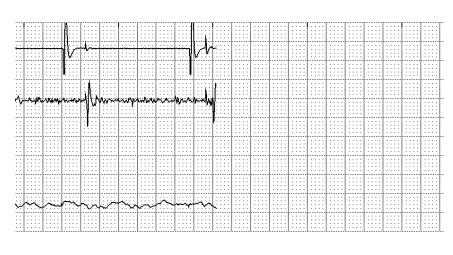



Clinician Signature:

