

Tachy Mode

ZOOM ® View™			Report Created 08 Nov 2016
	Selected Episodes Report		
KRÍZ, Karel			Last Office Interrogation
	Date of Birth	30 Aug 1954	31 Aug 2016
	Device	AUTOGEN X4 CRT-D G179/136339	Implant Date

Monitor + Therapy

12 Oct 2015

Event V-58: 01 Sep 2016 18:07

RhythmMatch™ Threshold: 94 %

VT Event Onset

Avg A Rate: 56 min<sup>-1</sup>

Avg V Rate: 248 min<sup>-1</sup>

Detection: Rhythm ID

Template: 27 Jul 2016 12:12

At V-Detect

Avg A Rate: 35 min<sup>-1</sup> Avg V Rate: 209 min<sup>-1</sup> Rate Zone: VT Stability: 55 ms V>A Rate: True


AFib: False

RhythmID Correlated: False RhythmMatch™: 28 % SRD Met: False

ATP Timeout: False

Attempt 1, Burst V ATP Elapsed Time: 00:00:04 ATP Information: Number of Bursts: 1

## Event Ended 00:00:17

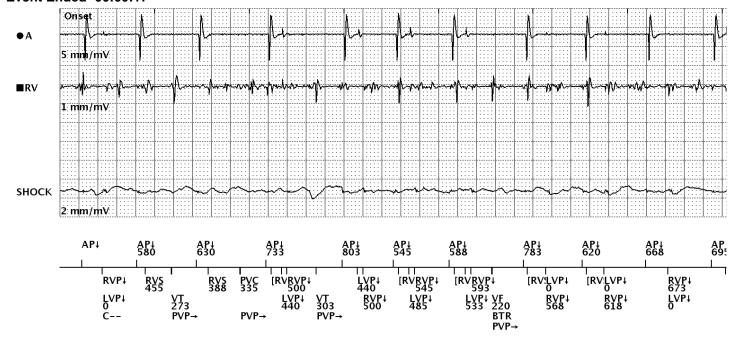



2868 Software Version: 3.07 G179 Firmware Version: E\_v1.02.00(2.01) © 2014


Boston Scientific Corporation
or its affiliates. All rights reserved.

Page 1 of 4

Clinician Signature:

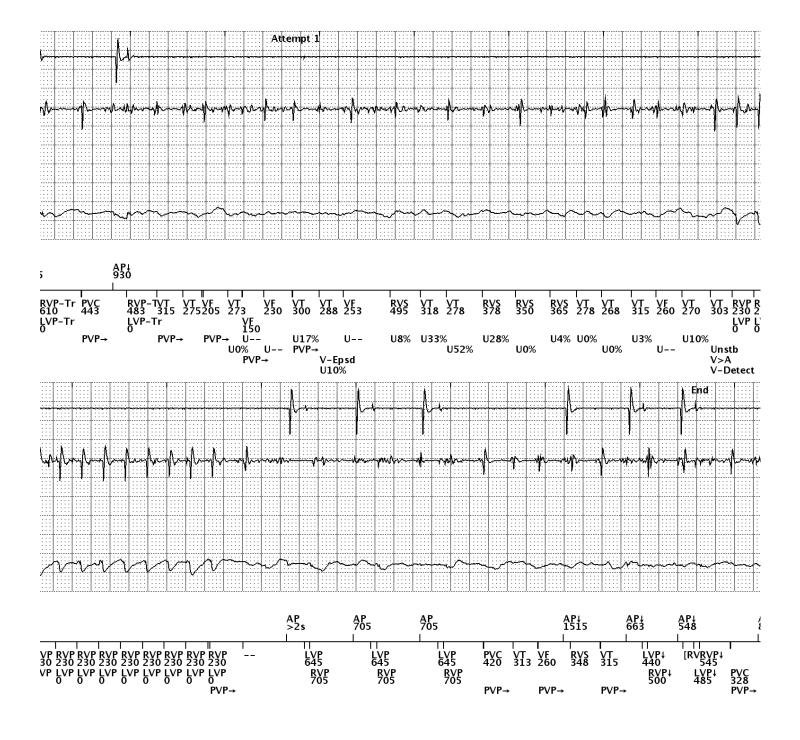

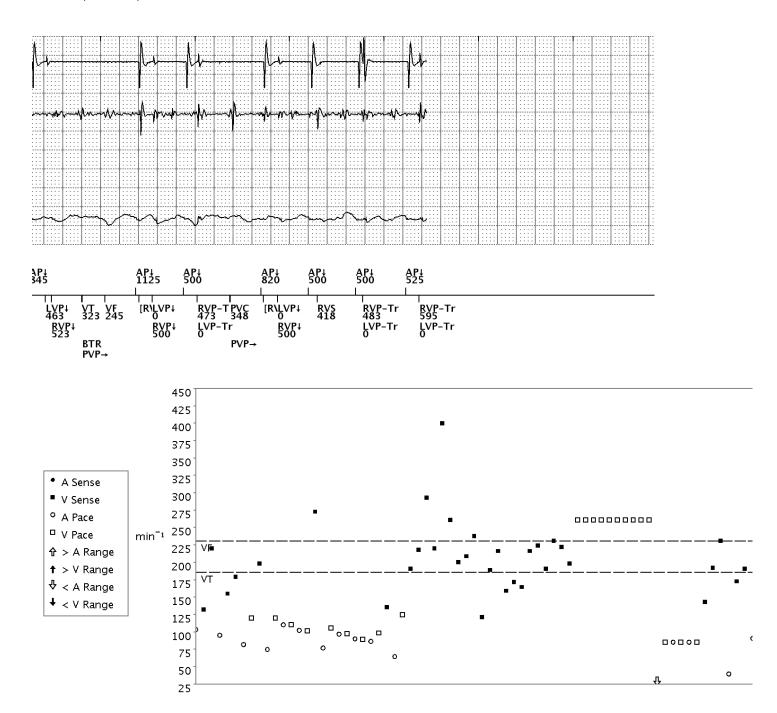

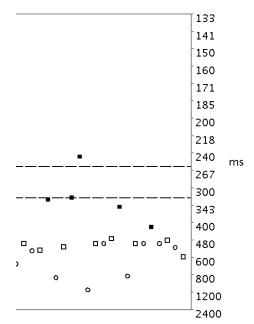

Clinician Signature: