

	ZOOM ® View™ Selected Episodes Report		Report Created 08 Nov 2016
	KRÍZ, Karel		Last Office Interrogation
	Date of Birth	30 Aug 1954	31 Aug 2016
	Device	AUTOGEN X4 CRT-D G179/136339	Implant Date
	Tachy Mode	Monitor + Therapy	12 Oct 2015

Event V-48: 01 Sep 2016 17:32

VF Event Onset
Avg A Rate: 100 min⁻¹
Avg V Rate: 308 min⁻¹
Detection: Rhythm ID

Template: 27 Jul 2016 12:12 RhythmMatch™ Threshold: 94 %

At V-Detect

Avg A Rate: 45 min⁻¹ Avg V Rate: 297 min⁻¹

Rate Zone: VF


Stability: (132 ms, Off) V>A Rate: (True, Off) AFib: (False, Off)

RhythmID Correlated: False RhythmMatch™: 0 % SRD Met: (False, Off) ATP Timeout: False Attempt 1, 36 J V Shock

Elapsed Time: 00:00:02 Aborted Attempt

No shock attempted due to fail to reconfirm



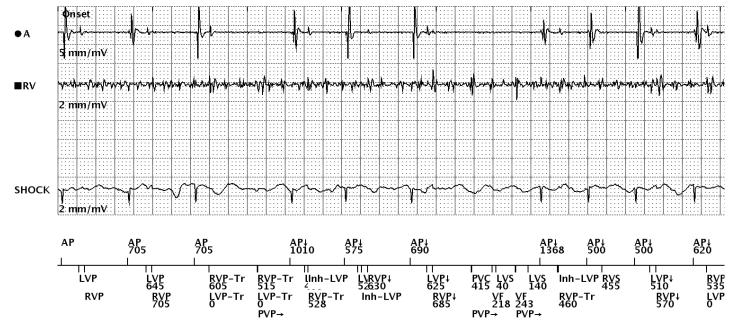


2868 Software Version: 3.07 G179 Firmware Version: E_v1.02.00(2.01) © 2014


Boston Scientific Corporation
or its affiliates. All rights reserved.

Page 1 of 4

Clinician Signature:

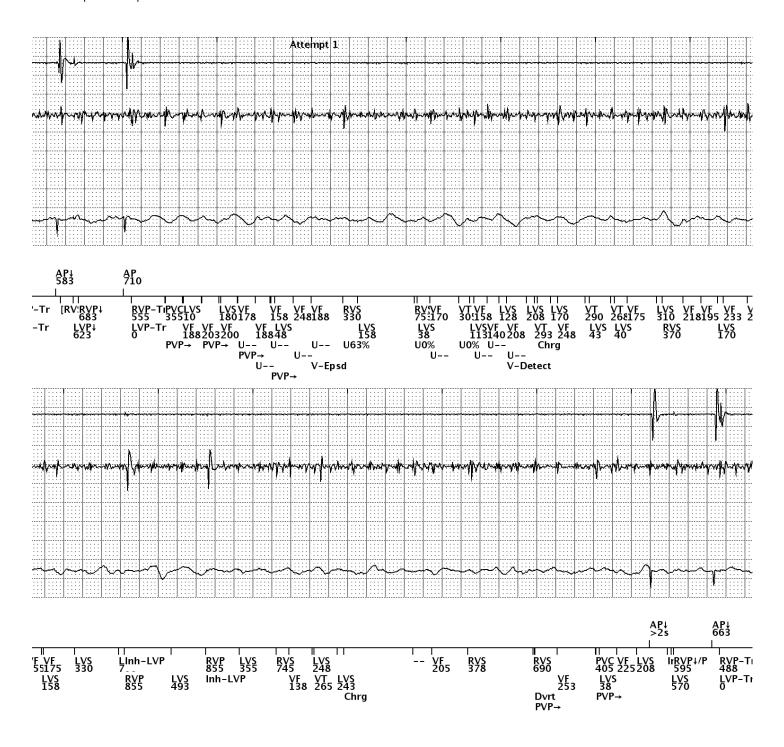





-Tr

LVP

Clinician Signature:

