

LATITUDE™ Programming System

**Real-time Log Report** Krajca 540702, Miroslav

Date of Birth N/R N/R N/R


Device CHARISMA CRT-D G324/500899 Tachy Mode

Monitor + Therapy

Report Created 23 Feb 2022

Last Office Interrogation

22 Feb 2022 Implant Date 22 Feb 2022

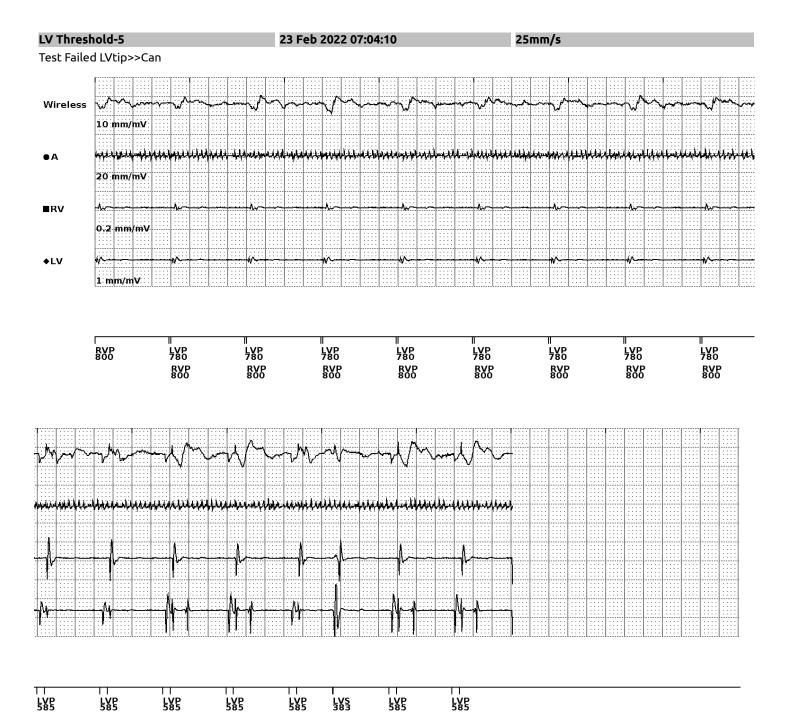

3868 Software Version: 1.10 G324 Firmware Version: H\_v1.00.00(1.01)

RVP 665

RVP 665

RVP 665

RVP 665

RVS 388

RVP 665

© 2014-2019 **Boston Scientific Corporation** or its affiliates. All rights reserved. Page 1 of 1

RVP 665

RVP 665

Clinician Signature: