

ZOOM ® View™		Report Created 08 Nov 2016	
Selected Episodes Report			
KRÍZ, Karel		Last Office Interrogation	
Date of Birth	30 Aug 1954	31 Aug 2016	
Device	AUTOGEN X4 CRT-D G179/136339	Implant Date	

12 Oct 2015

Monitor + Therapy

Tachy Mode

Event V-50: 01 Sep 2016 17:35

VF Event Onset
Avg A Rate: 69 min⁻¹
Avg V Rate: 296 min⁻¹
Detection: Rhythm ID
Template: 27 Jul 2016 12:12

RhythmMatch™ Threshold: 94 %

At V-Detect

Avg A Rate: 51 min⁻¹ Avg V Rate: 245 min⁻¹

Rate Zone: VF

Stability: (64 ms, Off) V>A Rate: (True, Off) AFib: (False, Off)


RhythmID Correlated: False RhythmMatch™: 0 % SRD Met: (False, Off) ATP Timeout: False

Attempt 1, 36 J V Shock Elapsed Time: 00:00:02

VF ATP delivered prior to shock

Shock Information: Charge Time: 5.8 s Lead Impedance: 53 Ω Lead Polarity: Initial

Event Ended 00:00:43

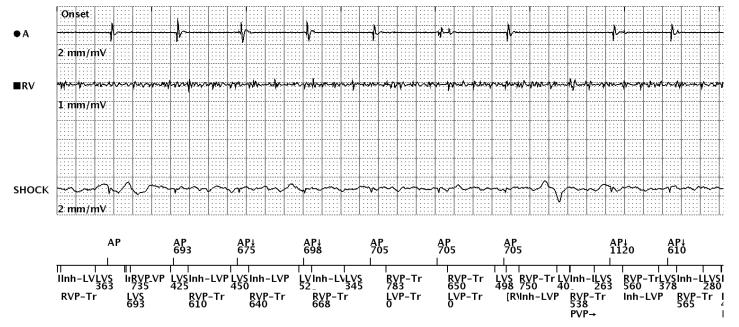


2868 Software Version: 3.07 G179 Firmware Version: E_v1.02.00(2.01) © 2014


Boston Scientific Corporation
or its affiliates. All rights reserved.

Page 1 of 4

Clinician Signature:



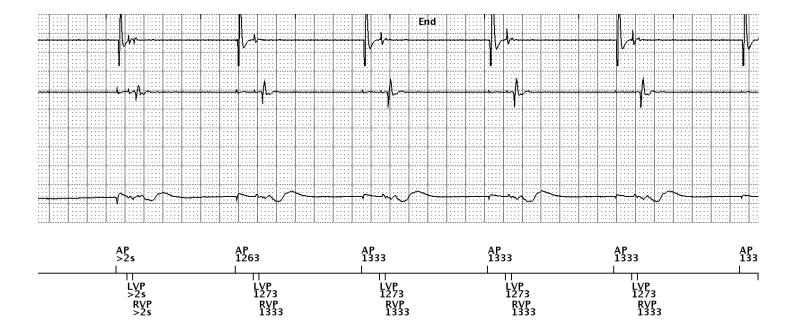

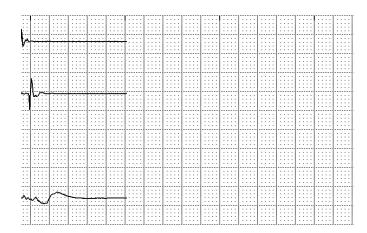

3 T LVP 1273 RVP 1333

2868 Software Version: 3.07 G179 Firmware Version: E_v1.02.00(2.01) © 2014

Boston Scientific Corporation
or its affiliates. All rights reserved.

Page 3 of 4

Clinician Signature:

