

**LATITUDE™ Programming System
Combined Follow-up Report**

Report Created 24 Jul 2021

Date of Birth N/R N/R N/R
Device ACCOLADE MRI L310/ 839486Last Office Interrogation
N/R
Implant Date
N/R**My Alerts**

There are no alerts to display.

Events Since Last Reset (23 Jul 2021)

24 Jul 2021 02:39 RV Auto

Battery OKApproximate time to explant: > 8 years
Magnet Rate 100 min⁻¹

One Year Remaining

Explant

**Leads Data****Implant****Previous Session****Most Recent**

N/R N/R N/R

Intrinsic Amplitude	N/R mV	N/R mV	13.3 mV@41 min ⁻¹
Pace Impedance	N/R Ω	N/R Ω	794 Ω
Pace Threshold	N/R V @ N/R ms	N/R	Auto 0.7 V @ 0.4 ms

POST completed. Test started at 23 Jul 2021 09:42**Settings****Tachy Settings**Tachy EGM Storage On
Detection Rate 160 min⁻¹**Brady Settings**

Mode	VVIR	Pacing Output	Auto 1.2 V @ 0.4ms
Lower Rate Limit	55 min ⁻¹	Sensitivity	AGC 0.6 mV
Maximum Sensor Rate	130 min ⁻¹	Leads Configuration (Pace/Sense)	Bipolar
Refractory	250 - 250 ms	Rate Adaptive Pacing	On
		Minute Ventilation	Passive
		Accelerometer	

Trends

Today's Activity: Program and Interrogate


R = Counter Reset
P = Program
I = Interrogate

Apr 21	May 21	Jun 21	Jul 21

Events

Apr 21	May 21	Jun 21	Jul 21

Activity Level

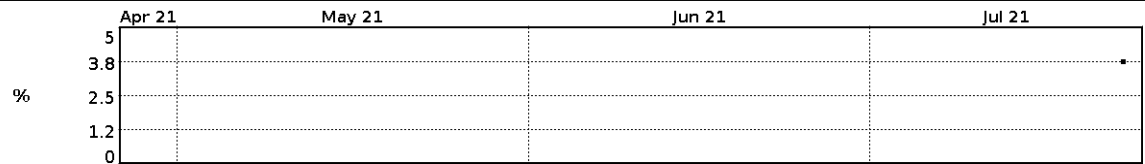

Heart Rate

Max
Mean
Min

min⁻¹

Apr 21	May 21	Jun 21	Jul 21

Respiratory Rate

Max
Median
Min

rpm

Apr 21	May 21	Jun 21	Jul 21


AP Scan

events/h

Apr 21	May 21	Jun 21	Jul 21


Intrinsic Amplitude

mV

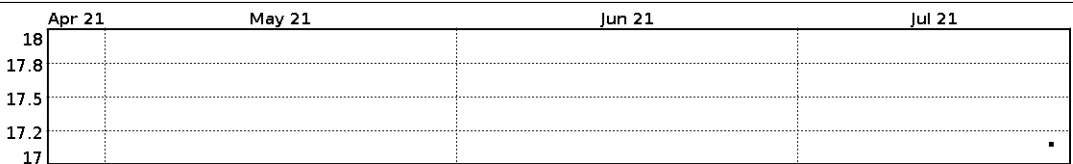


Pace Impedance

Ω

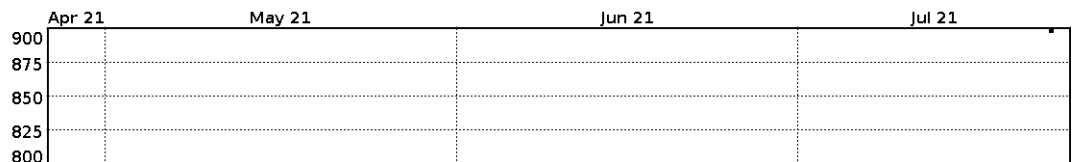


Pace Threshold

V

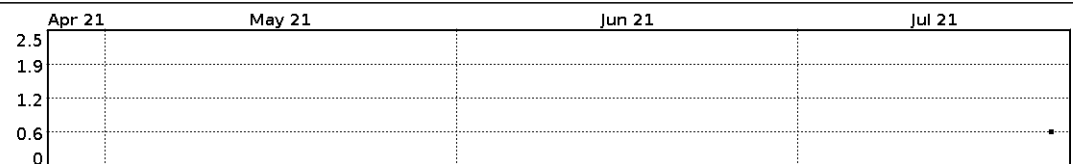

Tachy Counters		Since Last Reset	Device Totals
		23 Jul 2021	
Episode Counters			
Total Episodes		0	0
Tachy Episodes		0	0
Nonsustained Episodes		0	0
Brady Counters		Reset Before Last	Since Last Reset
		N/R day(s)	1 day(s)
		N/R to 23 Jul 2021	23 Jul 2021 to Today
Counters			
% Paced		0	74
Intrinsic Promotion			
Rate Hysteresis			
% Successful		0	0

Histograms Reset Before Last (N/R)

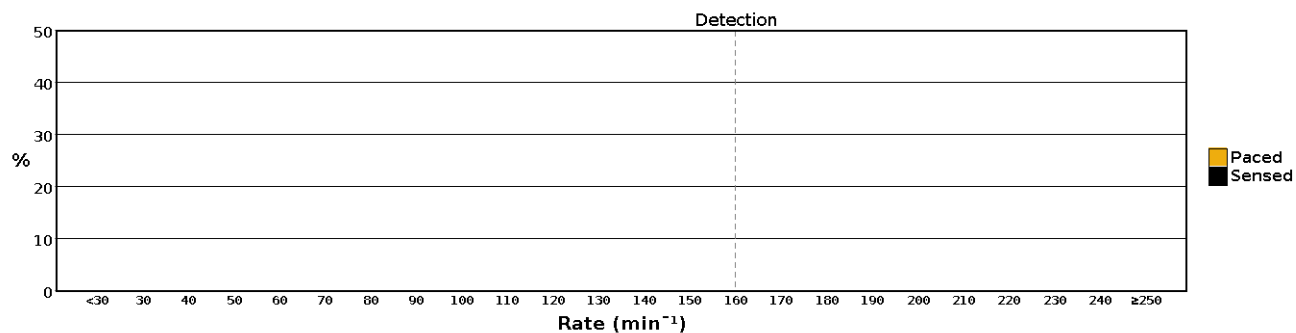

Histograms Since Last Reset (23 Jul 2021)

