

Date of Birth N/R N/R N/R
Device VITALIO MRI J276/102818

Last Office Interrogation
17 Jan 2017
Implant Date
N/R

My Alerts

There are no alerts to display.

Events Since Last Reset (29 May 2014)

31 Oct 2017 13:20 SVT (V<=A) at 154 min⁻¹
03 Feb 2015 11:48 SVT (V<=A) at 184 min⁻¹
See last page for full list of Events Since Last Reset.

Battery OK

Approximate time to explant: 7 years
Magnet Rate 100 min⁻¹

One Year Remaining

Explant



Leads Data

Implant
N/R N/R N/R

Previous Session

Most Recent

Atrial

Intrinsic Amplitude	N/R mV	3.5 mV	2.4 mV
Pace Impedance	N/R Ω	727 Ω	617 Ω
Pace Threshold	N/R V @ N/R ms	Auto 0.7 V @ 0.4 ms	Auto 0.6 V @ 0.4 ms

Ventricular

Intrinsic Amplitude	N/R mV	>25.0 mV	22.0 mV @ 87 min ⁻¹
Pace Impedance	N/R Ω	641 Ω	599 Ω
Pace Threshold	N/R V @ N/R ms	Auto 1.1 V @ 0.4 ms	Auto 1.1 V @ 0.4 ms

Settings

Ventricular Tachy Settings

Ventricular Tachy EGM Storage On
Detection Rate 160 min⁻¹

Atrial Tachy Settings

ATR Mode Switch 170 min⁻¹ DDI

Brady Settings

Mode DDDR
RYTHMIQ™ AAIR With
VVI Backup
Lower Rate Limit 55 min⁻¹
Maximum Tracking Rate 130 min⁻¹
Maximum Sensor Rate 130 min⁻¹
Paced AV Delay 80 - 180 ms
Sensed AV Delay 65 - 150 ms
A-Refractory (PVARP) 240 - 280 ms
V-Refractory (VRP) 230 - 250 ms

Pacing Output

Atrial Auto 2.0 V @ 0.4 ms
Ventricular 2.3 V @ 0.4 ms

Sensitivity

Atrial Fixed 0.5 mV
Ventricular Fixed 2.0 mV


Leads Configuration (Pace/Sense)

Atrial Bipolar
Ventricular Bipolar

Rate Adaptive Pacing


Minute Ventilation On
Accelerometer Passive

Trends

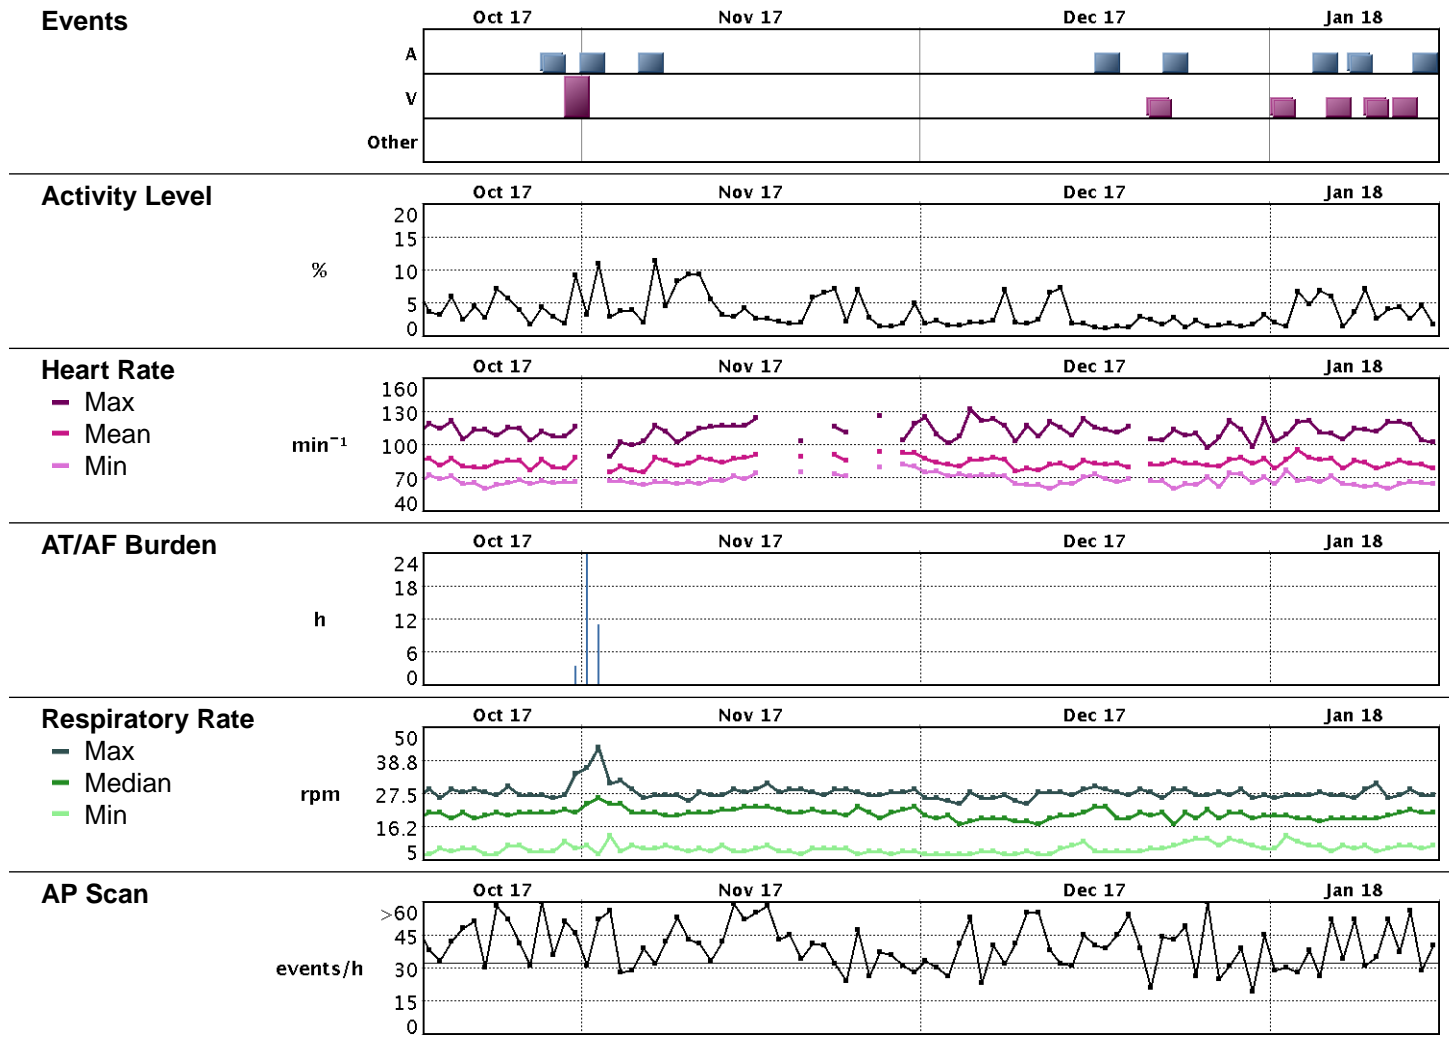


Trends (Continued)


P-Wave Amplitude




A Pace Impedance




A Pace Threshold




R-Wave (V) Amplitude



V Pace Impedance





V Pace Threshold





Ventricular Tachy Counters		Since Last Reset	Device Totals
		29 May 2014	
Ventricular Episode Counters			
Total Episodes		1.2K	1.2K
VT Episodes (V>A)		0	0
SVT Episodes (V<=A)		2	2
Nonsustained Episodes		1.2K	1.2K
Brady Counters		Reset Before Last	Since Last Reset
		N/R day(s)	1327 day(s)
		N/R to 29 May 2014	29 May 2014 to Today
Counters			
% A Paced		0	3
% V Paced		0	3
Intrinsic Promotion			
AV Search +			
% Successful		0	99
Rate Hysteresis			
% Successful		0	0
Atrial Arrhythmia			
% AT/AF		N/R	<1
(One Year of Data)			
Total Time in AT/AF (days)		N/R	1.6
(One Year of Data)			
Episodes by Duration			
< 1 minute		0	94
1 min - < 1 hr		0	0
1 hr - < 24 hr		0	0
24 hr - < 48 hr		0	1
> 48 hr		0	0
Total PACs		0	4.3M
Ventricular Counters			
Total PVCs		0	303.7K
Three or More PVCs		0	33

Histograms Reset Before Last (N/R)



Histograms Since Last Reset (29 May 2014)



All Events Since Last Reset (29 May 2014)

14 Jan 2018 17:47	RA Auto
12 Jan 2018 23:04	NonSustV at 168 min ⁻¹
12 Jan 2018 14:26	NonSustV at 149 min ⁻¹
12 Jan 2018 12:32	NonSustV at 147 min ⁻¹
12 Jan 2018 12:17	NonSustV at 197 min ⁻¹
12 Jan 2018 12:15	NonSustV at 159 min ⁻¹
12 Jan 2018 12:12	NonSustV at 149 min ⁻¹
11 Jan 2018 13:41	NonSustV at 159 min ⁻¹
11 Jan 2018 07:11	NonSustV at 144 min ⁻¹
11 Jan 2018 03:30	RYTHMIQ at 69 min ⁻¹
11 Jan 2018 03:27	RYTHMIQ at 64 min ⁻¹
10 Jan 2018 11:48	NonSustV at 156 min ⁻¹
10 Jan 2018 11:05	NonSustV at 146 min ⁻¹
10 Jan 2018 04:28	ATR at 64 min ⁻¹ , Avg V Rate in ATR: 67 min ⁻¹
09 Jan 2018 00:25	ATR at 102 min ⁻¹ , Avg V Rate in ATR: 90 min ⁻¹
07 Jan 2018 03:17	RYTHMIQ at 68 min ⁻¹
05 Jan 2018 21:36	ATR at 84 min ⁻¹ , Avg V Rate in ATR: 87 min ⁻¹
04 Jan 2018 02:52	RYTHMIQ at 65 min ⁻¹
04 Jan 2018 01:08	RYTHMIQ at 70 min ⁻¹
04 Jan 2018 00:41	RYTHMIQ at 78 min ⁻¹
02 Jan 2018 04:44	RYTHMIQ at 69 min ⁻¹
23 Dec 2017 14:44	ATR at 222 min ⁻¹ , Avg V Rate in ATR: 106 min ⁻¹
22 Dec 2017 03:54	RYTHMIQ at 65 min ⁻¹
22 Dec 2017 03:33	RYTHMIQ at 60 min ⁻¹
22 Dec 2017 03:29	RYTHMIQ at 60 min ⁻¹
17 Dec 2017 13:54	ATR at 86 min ⁻¹ , Avg V Rate in ATR: 90 min ⁻¹
07 Nov 2017 04:04	ATR at 88 min ⁻¹ , Avg V Rate in ATR: 105 min ⁻¹
01 Nov 2017 21:37	ATR at 81 min ⁻¹ , Avg V Rate in ATR: 103 min ⁻¹
31 Oct 2017 13:20	SVT (V<=A) at 154 min ⁻¹
30 Oct 2017 23:01	ATR at 303 min ⁻¹ , Avg V Rate in ATR: 98 min ⁻¹
29 Oct 2017 10:31	ATR at 98 min ⁻¹ , Avg V Rate in ATR: 84 min ⁻¹
22 Sep 2017 18:09	ATR at 86 min ⁻¹ , Avg V Rate in ATR: 85 min ⁻¹
19 Sep 2016 08:59	MRI
03 Feb 2015 11:48	SVT (V<=A) at 184 min ⁻¹