



ZOOM® View™

Combined Follow-up Report

Report Created 02 Jul 2014

Date of Birth N/R N/R N/R
Device INVIVE W173/118030Last Office Interrogation
N/R
Implant Date
N/R

My Alerts

There are no alerts to display.

Events Since Last Reset (02 Jul 2014)

There are no events to display.

Battery OK

Approximate time to explant: > 7 years
Magnet Rate 100 min⁻¹

One Year Remaining

Explant



Leads Data

Implant
N/R N/R N/R

Previous Session

Most Recent

Atrial

Intrinsic Amplitude	N/R mV	N/R mV	N/R mV
Pace Impedance	N/R Ω	N/R Ω	>2000 Ω
Pace Threshold	N/R V @ N/R ms	N/R	

Right Ventricular

Intrinsic Amplitude	N/R mV	N/R mV	PVC mV @ N/R min ⁻¹
Pace Impedance	N/R Ω	N/R Ω	874 Ω
Pace Threshold	N/R V @ N/R ms	N/R	Auto 0.5 V @ 0.4 ms

Left Ventricular

Intrinsic Amplitude	N/R mV	N/R mV	PVC mV
Pace Impedance	N/R Ω	N/R Ω	1347 Ω
Pace Threshold	N/R V @ N/R ms	N/R	0.8 V @ 0.4 ms

Settings

Ventricular Tachy Settings

Ventricular Tachy EGM Storage	On
Detection Rate	160 min ⁻¹

Brady/CRT Settings

Mode	VVIR	Pacing Output	
Lower Rate Limit	80 min ⁻¹	Right Ventricular	Auto 2.0 V @ 0.4 ms
Maximum Sensor Rate	130 min ⁻¹	Left Ventricular	3.0 V @ 0.4 ms
RV-Refractory (RVRP)	230 - 250 ms	Sensitivity	
LV-Refractory (LVRP)	250 ms	Atrial	Fixed 0.75 mV
Ventricular Pacing Chamber	BiV	Right Ventricular	Fixed 2.5 mV
LV Offset	-40 ms	Left Ventricular	Fixed 2.5 mV
		Leads Configuration (Pace/Sense)	
		Atrial	--/Bipolar
		Right Ventricular	Bipolar
		Left Ventricular	LVtip>>LVring
		Rate Adaptive Pacing	
		Accelerometer	On

Trends

Events		Apr 14	May 14	Jun 14
A				
RV				
Other				

Activity Level		Apr 14	May 14	Jun 14
%				

Heart Rate		Apr 14	May 14	Jun 14
Max				
Mean				
Min				
min ⁻¹				

SDANN		Apr 14	May 14	Jun 14
ms				

HRV Footprint		Apr 14	May 14	Jun 14
%				

Autonomic Balance Monitor		Apr 14	May 14	Jun 14

Atrial Burden		Apr 14	May 14	Jun 14
h				

Respiratory Rate		Apr 14	May 14	Jun 14
Max				
Median				
Min				
rpm				

AP Scan		Apr 14	May 14	Jun 14
events/h				

Trends (Continued)

P-Wave Amplitude

	Apr 14	May 14	Jun 14
mV			

A Pace Impedance

	Apr 14	May 14	Jun 14
Ω			

R-Wave (RV) Amplitude

	Apr 14	May 14	Jun 14
mV			

RV Pace Impedance

	Apr 14	May 14	Jun 14
Ω			

RV Pace Threshold

	Apr 14	May 14	Jun 14
V			

R-Wave (LV) Amplitude


	Apr 14	May 14	Jun 14
mV			

LV Pace Impedance


	Apr 14	May 14	Jun 14
Ω			

Ventricular Tachy Counters		Since Last Reset	Device Totals
		02 Jul 2014	
Ventricular Episode Counters			
Total Episodes		0	0
VT Episodes (V>A)		0	0
SVT Episodes (V<=A)		0	0
Nonsustained Episodes		0	0
Brady/CRT Counters		Reset Before Last	Since Last Reset
		N/R	02 Jul 2014
Counters			
% A Paced		0	0
% RV Paced		0	4
% LV Paced		0	3
Intrinsic Promotion			
Rate Hysteresis			
% Successful		0	0
Atrial Burden			
Atrial Burden %		N/R	N/R
Episodes by Duration			
< 1 minute		0	0
1 min - < 1 hr		0	0
1 hr - < 24 hr		0	0
24 hr - < 48 hr		0	0
> 48 hr		0	0
Total PACs		0	19
Ventricular Counters			
Total PVCs		0	422
Three or More PVCs		0	9

Histograms Reset Before Last (N/R)



Histograms Since Last Reset (02 Jul 2014)

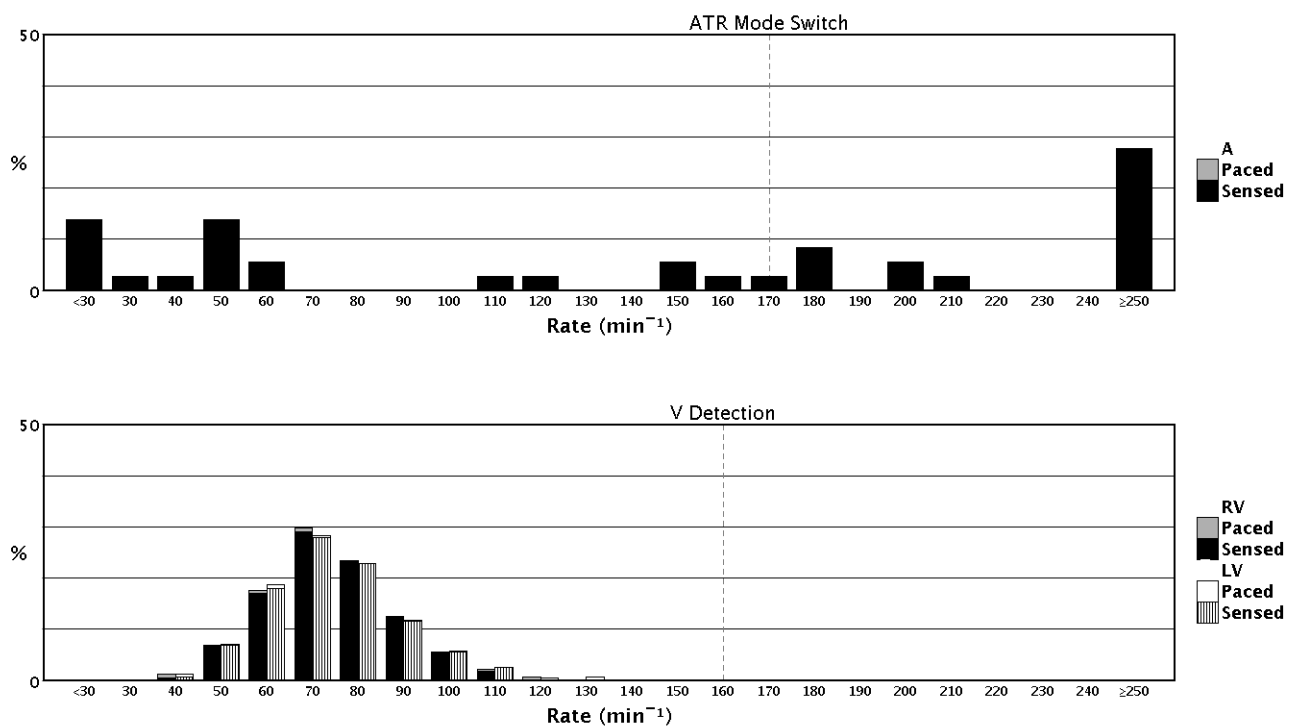

Heart Rate Variability

Last Measured:

HRV data unavailable because device was reprogrammed in the last 24 hours.

Reference:

HRV data unavailable because device was reprogrammed in the last 24 hours.