



ZOOM® View™

Combined Follow-up Report

Report Created 04 Jun 2014

Date of Birth N/R N/R N/R
Device VITALIO MRI J275/101893

Last Office Interrogation
N/R
Implant Date
N/R

My Alerts

There are no alerts to display.

Events Since Last Reset (02 Jun 2014)

04 Jun 2014 04:17 NonSust at 305 min⁻¹

Battery OK

Approximate time to explant: > 8 years
Magnet Rate 100 min⁻¹

One Year Remaining

Explant



Leads Data

Implant

Previous Session

Most Recent

N/R N/R N/R

Intrinsic Amplitude	N/R mV	N/R mV	24.9 mV @ 48 min ⁻¹
Pace Impedance	N/R Ω	N/R Ω	616 Ω
Pace Threshold	N/R V @ N/R ms	N/R	Auto 0.6 V @ 0.4 ms

Settings


Tachy Settings

Tachy EGM Storage On
Detection Rate 160 min⁻¹

Brady Settings


Mode	VVIR	Pacing Output	Auto 1.1 V @ 0.4 ms
Lower Rate Limit	55 min ⁻¹	Sensitivity	Fixed 2.5 mV
Maximum Sensor Rate	115 min ⁻¹	Leads Configuration (Pace/Sense)	Unipolar/Bipolar
Refractory	250 - 250 ms	Rate Adaptive Pacing	On
		Minute Ventilation	Passive
		Accelerometer	

Trends

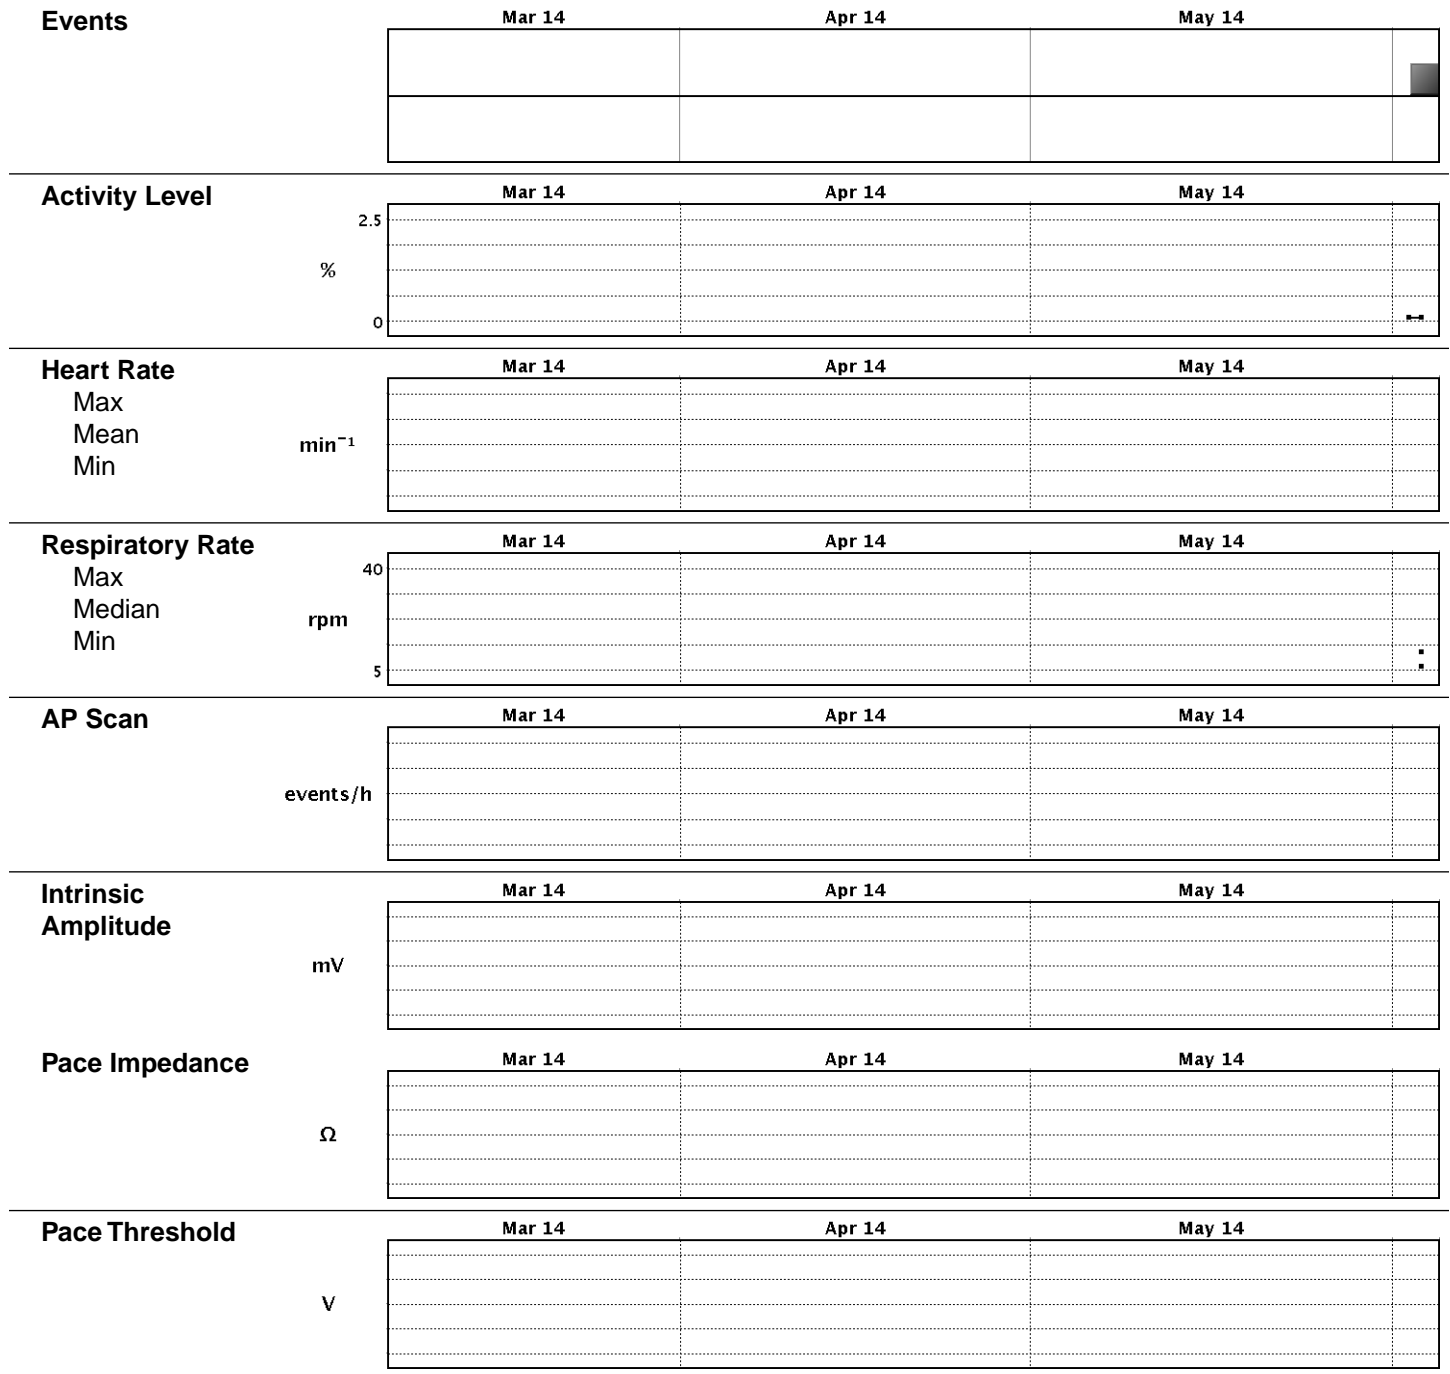

Tachy Counters		Since Last Reset	Device Totals
		02 Jun 2014	
Episode Counters			
Total Episodes		1	1
Tachy Episodes		0	0
Nonsustained Episodes		1	1
Brady Counters		Reset Before Last	Since Last Reset
		N/R	02 Jun 2014
Counters			
% Paced		0	74
Intrinsic Promotion			
Rate Hysteresis			
% Successful		0	0

Histograms Reset Before Last (N/R)

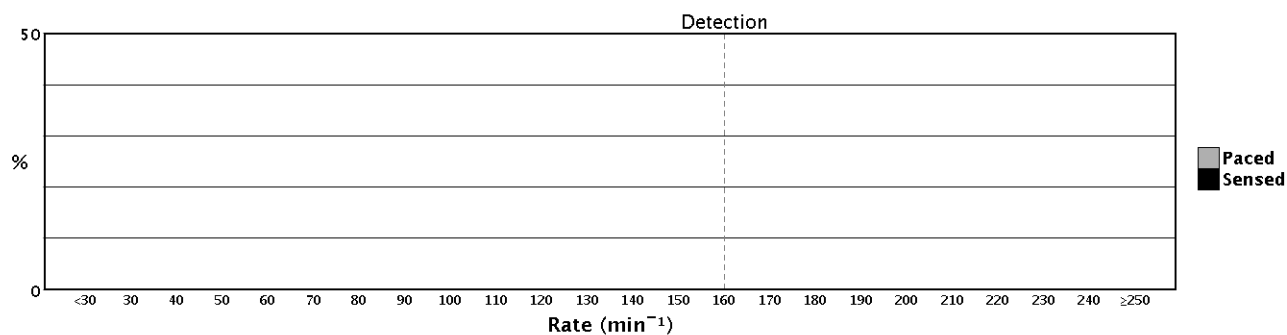

Histograms Since Last Reset (02 Jun 2014)

