
TNBC

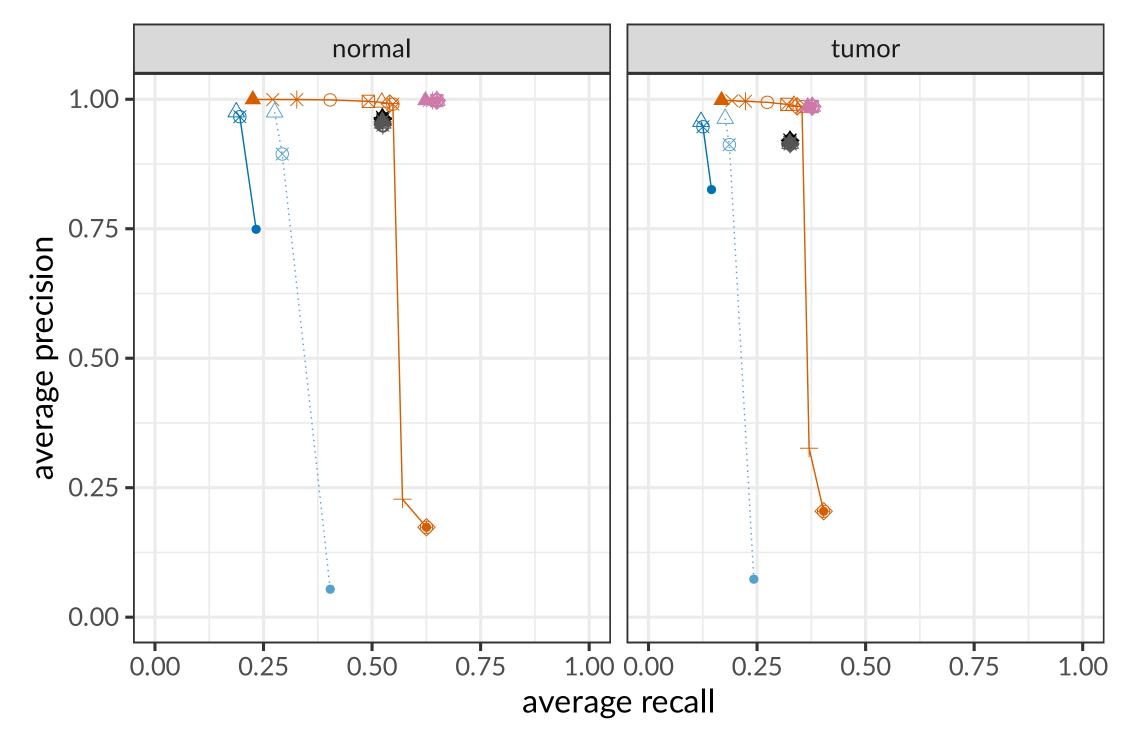

software

- MonoVar default
- MonoVar no consensus
- ProSolo default
- ProSolo imputation^{-b}
- **SCAN-SNV** sensitive
- SCcaller default dbsnp
- SCcaller sensitive dbsnp
- SCIPhI default
- SCIPhI sensitive^{-b}

threshold used

- 1e-06
- 1e-05
- 1e-04
- 0.001
- 0.005
- 0.01
- 0.02
- 0.05
- 0.1
- 0.2 0.5