
IL-11 and IL-12

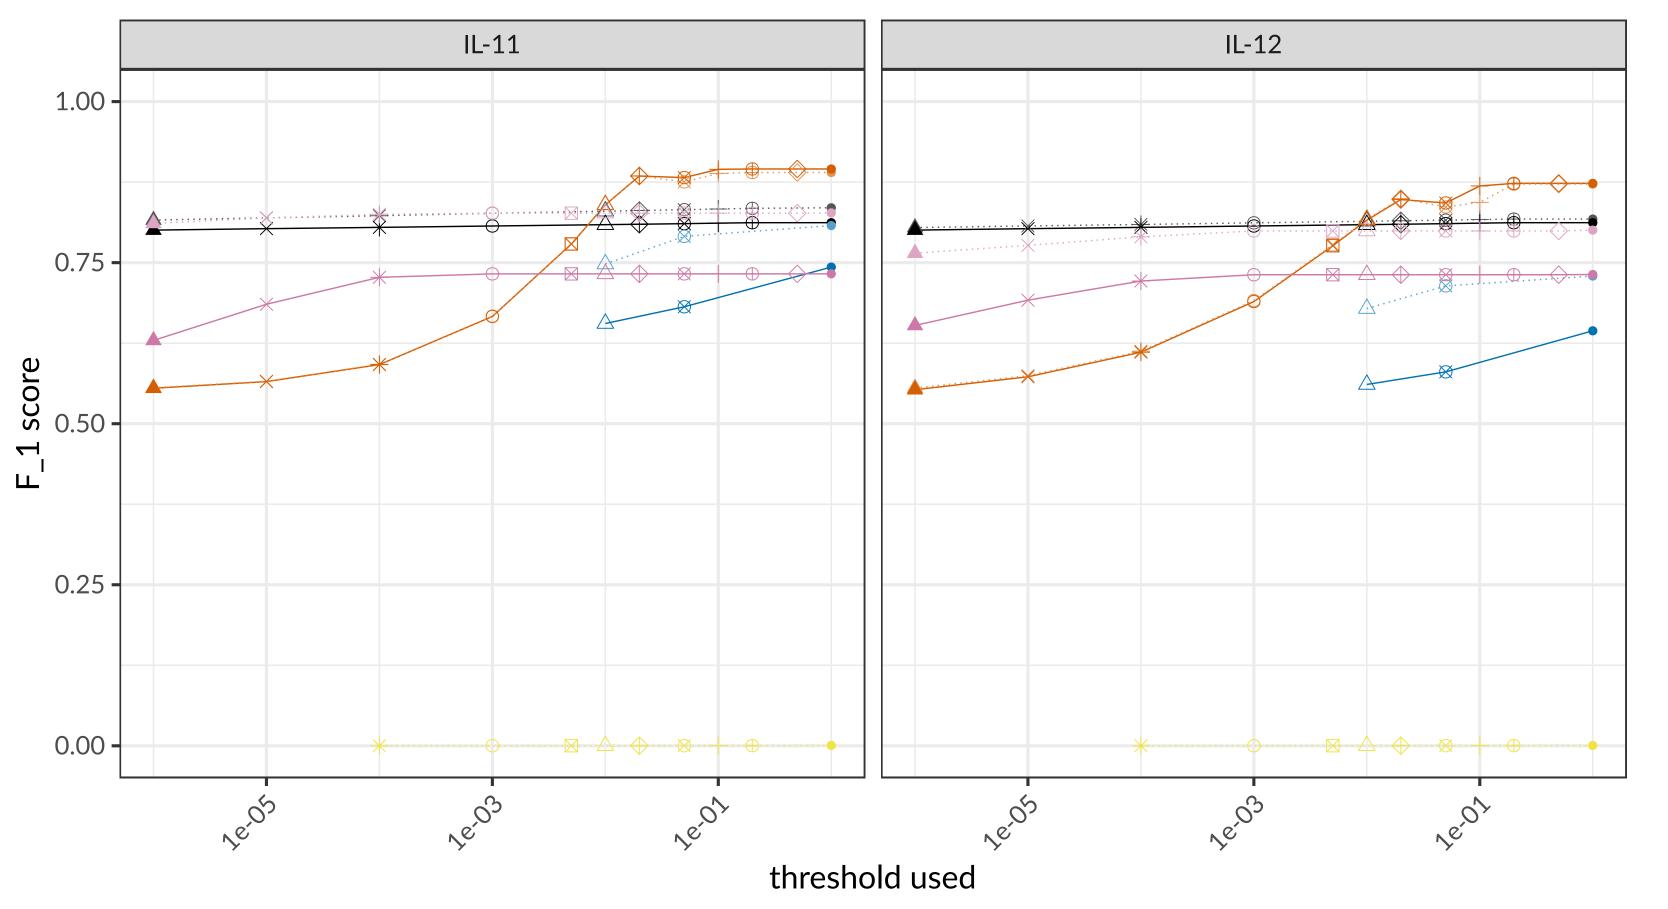

software

- MonoVar default

- MonoVar default
 MonoVar no consensus
 ProSolo default
 ProSolo imputation
 SCAN-SNV sensitive
 SCcaller default dbsnp
 SCcaller sensitive dbsnp
 SCIPhI default
 SCIPhI sensitive

threshold

- ▲ 1e-06 × 1e-05 * 1e-04
- 0.001
- 0.005
- 0.01
- 0.02 0.05
- \oplus
- 0.1 0.2 0.5 \Diamond