
IL-11 and IL-12

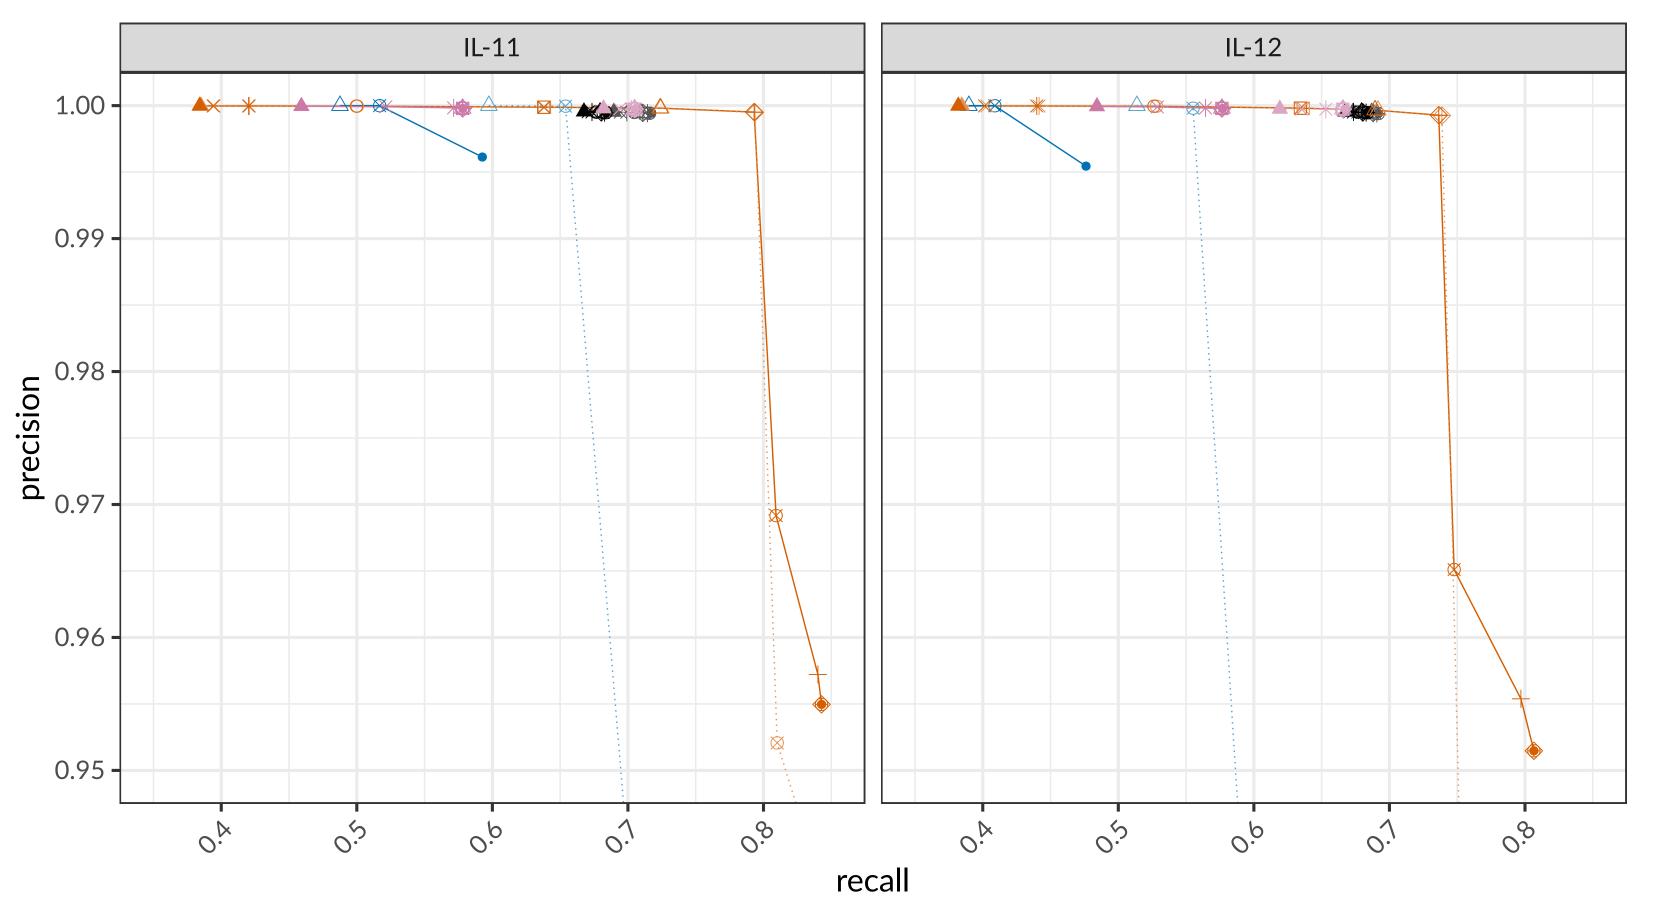

software

- MonoVar default
- MonoVar no consensus

- ProSolo default
 ProSolo imputation
 SCAN-SNV sensitive
 SCcaller default dbsnp
 SCcaller sensitive dbsnp
 SCIPhI default
 SCIPhI sensitive

threshold

- ▲ 1e-06 × 1e-05
- * 1e-04
- 0.001
- 0.005
- 0.01 0.02 0.05 0.1 0.2 0.5 1
- +⊕♦