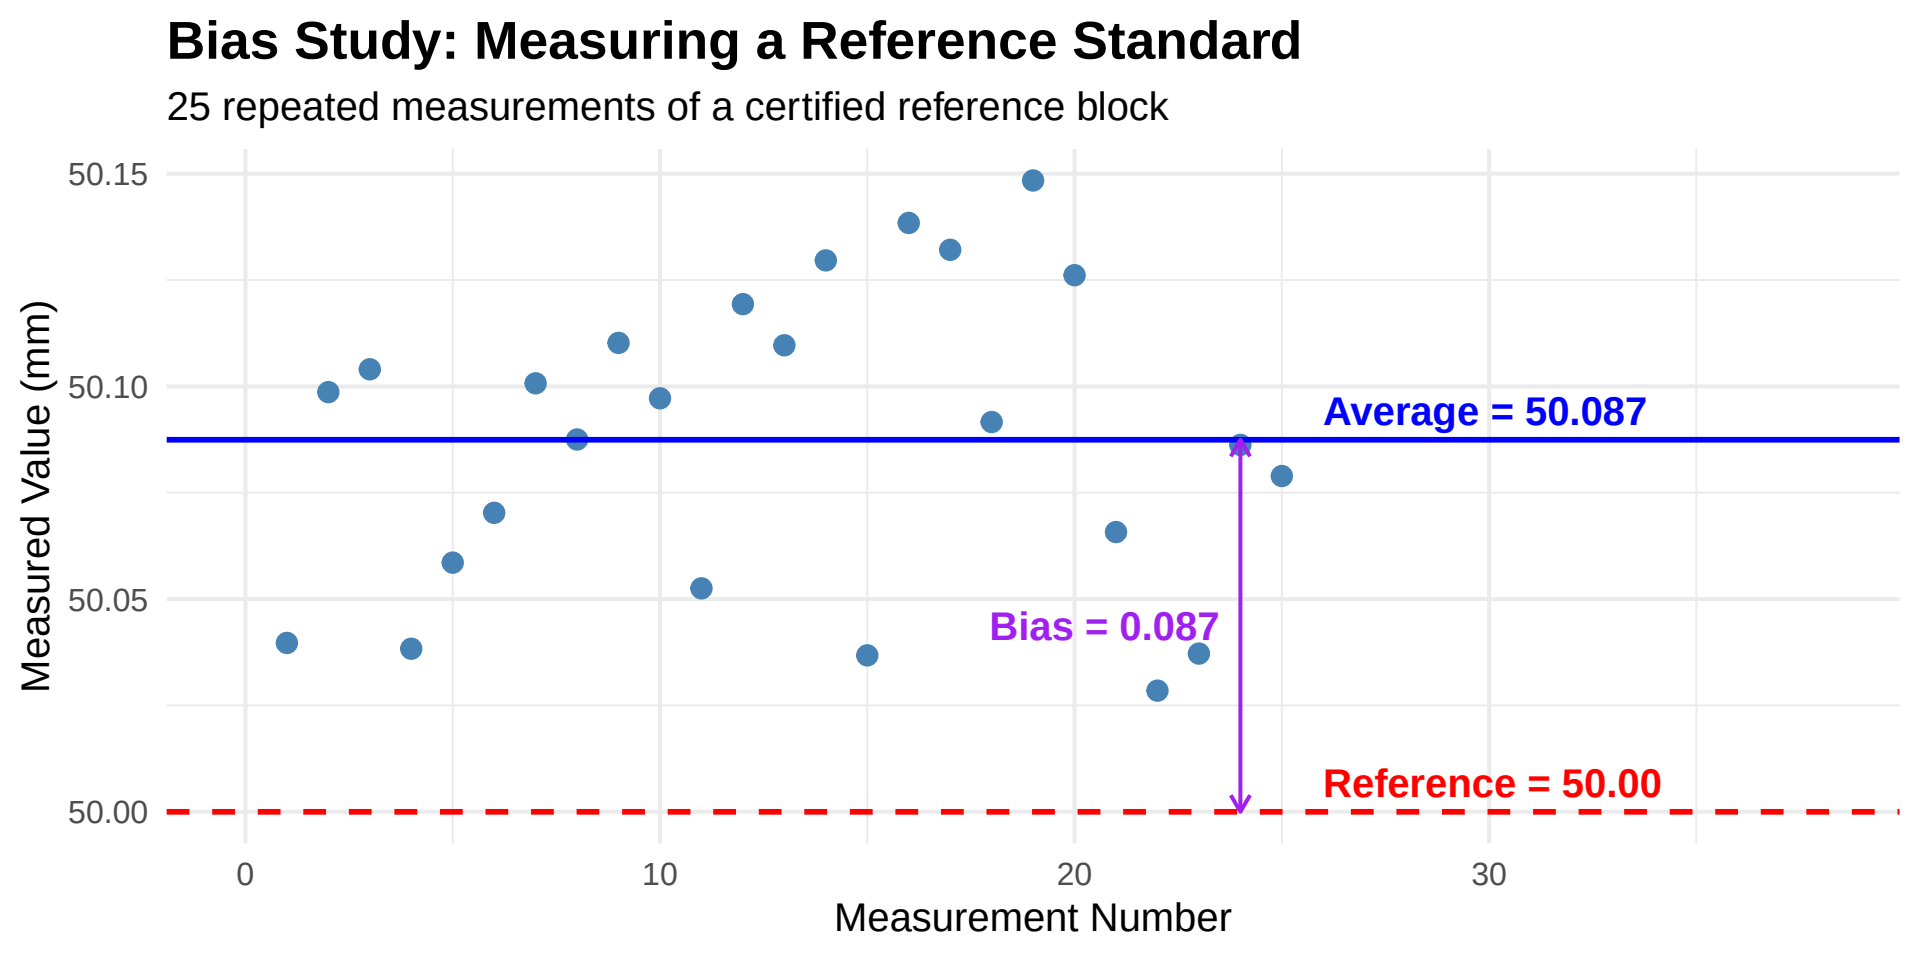
Bias Study: Measuring a Reference Standard
25 repeated measurements of a certified reference block
Measured Value (mm)
50.15
50.10
50.05
50.00
0
10
20
30
Measurement Number
Average = 50.087
Bias = 0.087
Reference = 50.00