

# Certificate of Analysis

Part Number:	090-201	Serial Number:	
Product Name:	Maurice cIEF-65 Cartridge	Date of Manufacture:	

This product was tested on a Maurice system with system suitability and passed all physical and functional test criteria.

## Test Methods

Analysis of Maurice cIEF-65 Cartridge on Maurice or Maurice C. systems. All tests were performed using ProteinSimple's Maurice cIEF System Suitability. Figure 1, representative electropherogram collected in absorbance mode, for pI markers 3.38, 5.85, 6.14, 9.99, and 10.17. Figure 2, representative electropherogram collected in fluorescence mode, for the same set of pI markers.

Figure 1. Absorbance


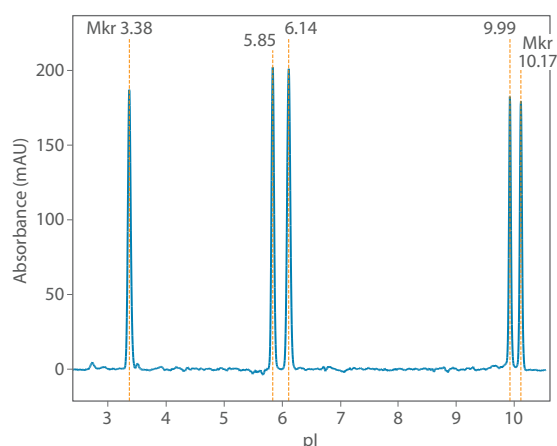


Figure 2. Fluorescence

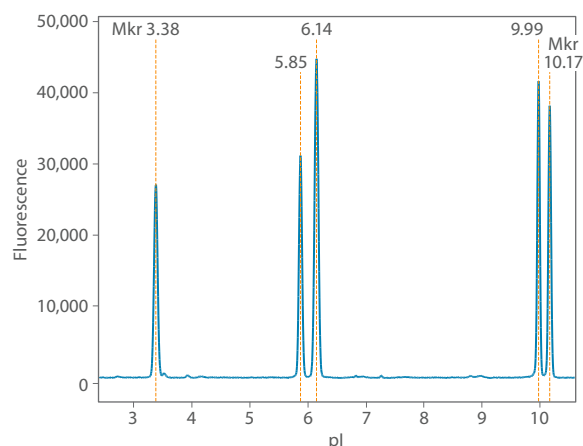

## Acceptance Results

PARAMETER	ACCEPTANCE CRITERIA	PASS/FAIL
pI Range	pI 3.38, 5.85, 6.14, 9.99, and 10.17 markers observed	Pass
Resolution 6.14 (Fluorescence)	$\geq 2.10$	Pass
Resolution 10.17 (Fluorescence)	$\geq 1.70$	Pass

Reviewed and Approved:

Hooi Tan  
Sr. Quality Manager

Date:



Toll-free: (888) 607-9692  
Tel: (408) 510-5500  
info@proteinsimple.com  
proteinsimple.com

3001 Orchard Parkway  
San Jose, CA 95134  
USA