

Product Description

Part Number #	101-0064	Serial Number	
Product Name	Maurice iCIEF 400 Cartridge	Date of Manufacture	
		Batch No.	

This product was tested on a Maurice system with system suitability and passed all physical and functional test criteria.

Test Methods

Analysis of Maurice iCIEF Cartridge on Maurice or Maurice C. systems. All tests were performed using ProteinSimple's Maurice iCIEF System Suitability. FIGURE 1, representative electropherogram collected in absorbance mode, for pI markers 3.38, 5.85, 6.14, 9.99, and 10.17. FIGURE 2, representative electropherogram collected in fluorescence mode, for the same set of pI markers.

Figure 1. Absorbance


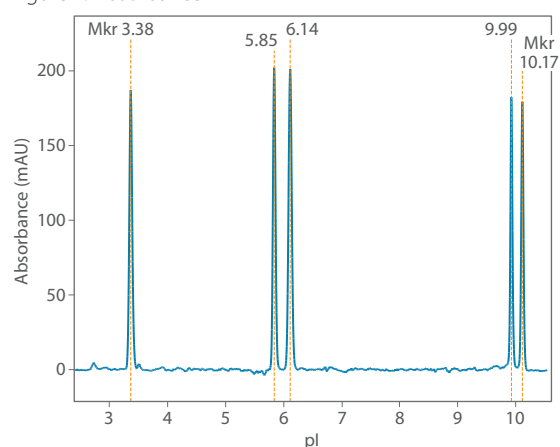


Figure 2. Fluorescence

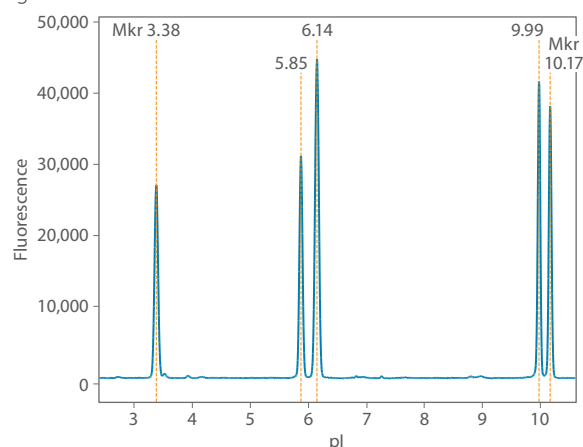

ACCEPTANCE RESULTS

PARAMETER	ACCEPTANCE CRITERIA	PASS/FAIL
pI Range	pI 3.38, 5.85, 6.14, 9.99, and 10.17 markers observed	Pass
Resolution 6.14 (Fluorescence, 10s exposure)	≥ 2.10	Pass
Resolution 10.17 (Fluorescence, 10s exposure)	≥ 1.70	Pass

Reviewed and Approved:

Hooi Tan
Sr. Quality Manager
Date:

Bio-Techne® | R&D Systems™ Novus Biologicals™ Tocris Bioscience™ ProteinSimple™ ACD™

ProteinSimple Proprietary & Confidential Information

Template Q51-0198 / Rev A

Page 1 of 1

Q51-0208 / Rev A