

## Maurice CE-SDS PLUS Cartridge


Part Number	090-157	Serial Number	
Product Name	Maurice CE-SDS PLUS Cartridge	Date of Manufacture	
		Expiration Date	

This product was tested on a Maurice system and passed all physical and functional test criteria.

### Test Methods

Analysis of Maurice CE-SDS PLUS Cartridge on Maurice or Maurice S. systems. All tests were performed using ProteinSimple's reduced IgG standard. **Figure 1**, representative electropherogram for Reduced IgG standard, Peaks: internal standard (IS, 10KD), light chain (LC), non-glycosylated heavy chain (NGHC), glycosylated heavy chain (HC).

Figure 1.

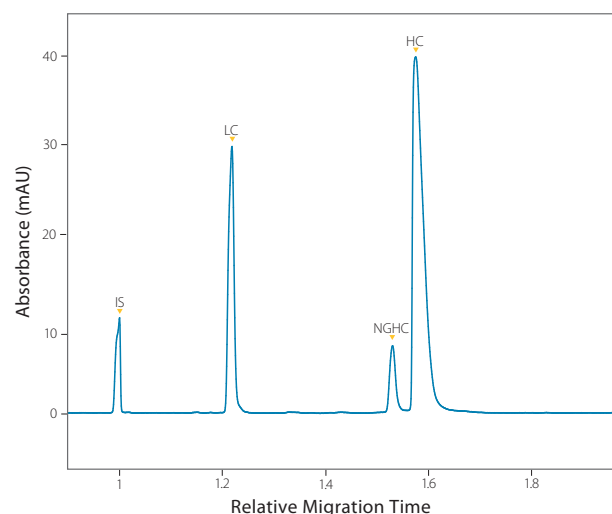

### ACCEPTANCE RESULTS

Parameter	Acceptance Criteria	Pass/Fail
Resolution, HC (Reduced Sample)	$\geq 1.50$	Pass
Peak Height, HC (Reduced Sample)	$\geq 20.0$ mAU	Pass

Reviewed and Approved:

Hooi Tan  
Sr. Quality Manager  
Date: