

CE-SDS PLUS 50 Cartridge


Part Number	101-0069	Serial Number	
Product Name	CE-SDS PLUS 50 Cartridge	Date of Manufacture	
		Expiration Date	
		Batch No.	

This product was tested on a Maurice system with system suitability and passed all physical and functional test criteria.

Test Methods

Analysis of CE-SDS PLUS 50 Cartridge on Maurice or Maurice S. systems. All tests were performed using ProteinSimple's reduced IgG standard. FIGURE 1, representative electropherogram Reduced IgG standard, Peaks: internal standard (IS, 10KD), light chain (LC), non-glycosylated heavy chain (NGHC), glycosylated heavy chain (HC).

Figure 1

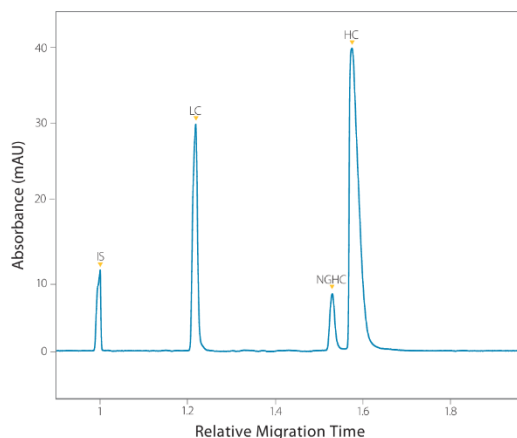

ACCEPTANCE RESULTS

PARAMETER	ACCEPTANCE CRITERIA	PASS/FAIL
Resolution, HC (Reduced Sample)	≥ 1.50	Pass
Peak Height, HC (Reduced Sample)	≥ 20.0 mAU	Pass

Reviewed and Approved:

Hooi Tan
Sr. Quality Manager
Date: