
Power Report 2025-10-09

Alternative: NORMALGENERATOR | (α): 0.01


Test	200	400	600	800	1000
KS	0.000	0.000	0.000	0.000	0.000
AD	0.988	0.987	0.985	0.991	0.995



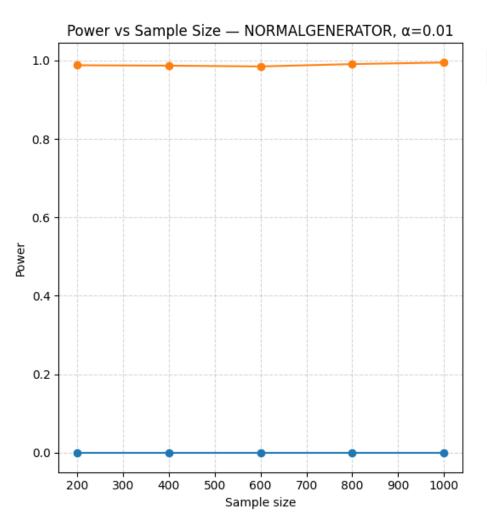

Alternative: NORMALGENERATOR | (α): 0.05

Test	200	400	600	800	1000
KS	0.000	0.000	0.000	0.000	0.000
AD	0.947	0.946	0.944	0.949	0.960

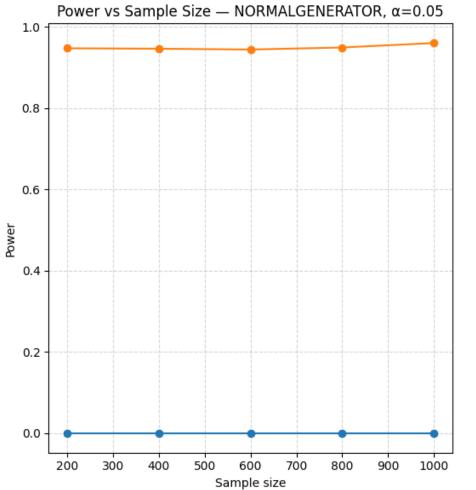




Alternative: NORMALGENERATOR | (α): 0.1

Test	200	400	600	800	1000
KS	0.000	0.000	0.000	0.000	0.000
AD	0.891	0.898	0.896	0.888	0.909



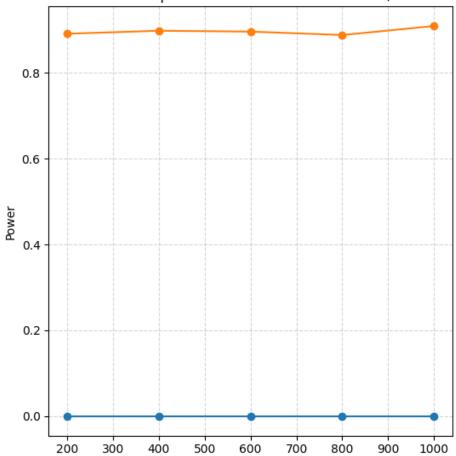

Sample size

KS_NORMALITY_GOODNESS_OF_FIT

AD_NORMALITY_GOODNESS_OF_FIT