




## Meeco Moisture Analyzer

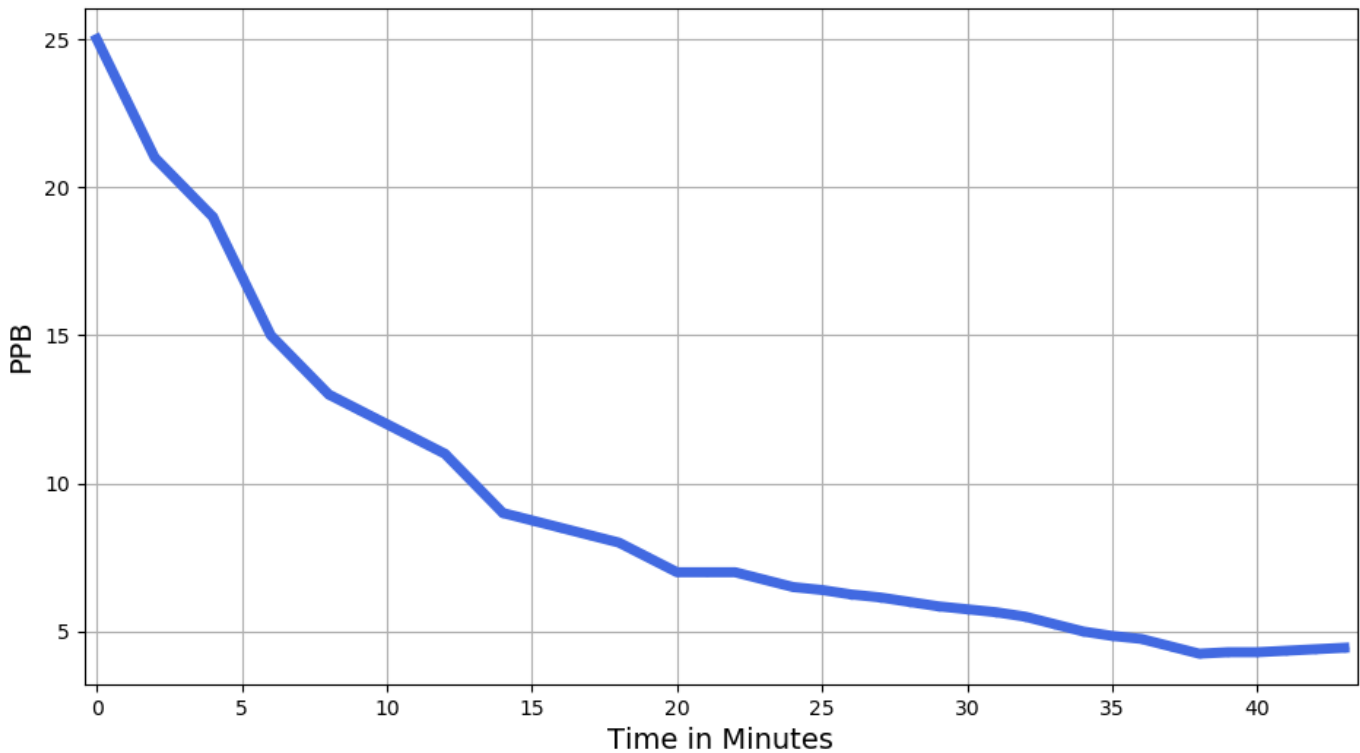

Client:

TFS

Location:

TFS WAr

Instrument Serial #:

1337-45-8

Calibration Date:

07/2019

Specification:

10 above source

Instrument Flow:

2.1 SLPM

Test Gas: Argon

Source Gas: 39

Test Point ID: TFS WAr IN CLEANROOM

Technician: JCH

System Flow: 2.1 SLPM

Start Time: 2020-02-13 14:54:56

Stop Time: 2020-02-13 14:55:16

Maximum: 25.0 PPB

Average: 9.23 PPB

Final: 4.45 PPB

Comments: TFS WAr INSIDE CLEANROOM; FURTHEST POINT

Approval: