

Approved by	Checked by	Prepared by
Kato Shunichi		Nhu Dinh Duy

FLOW CHART TO CALIBRATION,CALIBRATION PROCEDURE

Confidential : Canon internal use only

LBP Material Quality Assurance	Issued No LBPMQA-FA-038	Revision 01
--------------------------------	----------------------------	-----------------------

Quy trình hiệu chuẩn thiết bị phòng MQA


Hiệu chuẩn định kỳ

Hiệu chuẩn đặc biệt

Yêu cầu từ MQA

Nhận list hiệu chuẩn từ phòng PQA

Tập hợp thiết bị

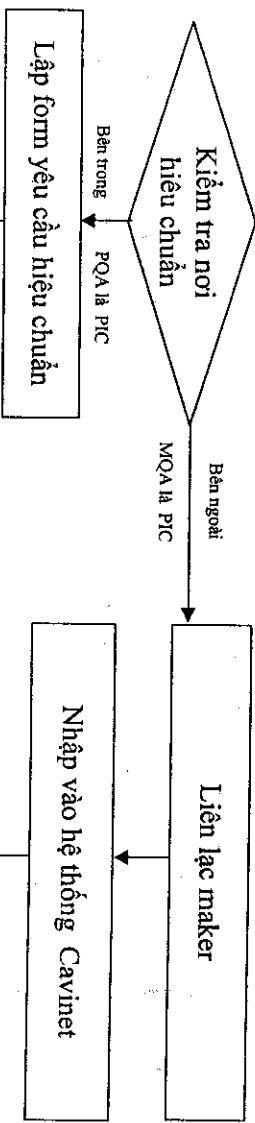


Nội dung công việc

Ver :01	
Approval by :	Issued by :

⇒	+ List hiệu chuẩn nhận từ PQA hàng tháng (qua Email)
⇒	+ PQA : Mr Quy Anh , Mr Thai
⇒	+ MQA : Mr Duy , Mr Tuan
⇒	+ MQA gửi thiết bị hiệu chuẩn cho phòng PQA trước ngày hiệu chuẩn là 1 ngày
⇒	+ MQA : Ms Tuyet , Ms Luong
⇒	+ PQA : Mr Quy Anh , Mr Thai
⇒	+ Yêu cầu maker gửi bản báo giá đến MQA
⇒	+ Xác nhận ngày hiệu chuẩn
⇒	+ Nhập thiết bị hiệu chuẩn vào hệ thống Cavinet
⇒	+ In Purchase approval sheet rồi xin chữ ký Manager , GM, FM..
⇒	+ Gửi Purchase approval cho phòng Pur
⇒	+ Maker đến Canon để hiệu chuẩn
⇒	+ Nhận dữ liệu hiệu chuẩn
⇒	+ Dán tem chứng nhận hiệu chuẩn lên thiết bị
⇒	+ Copy dữ liệu hiệu chuẩn cho phòng PQA (Mr Quy Anh)
⇒	+ In kết quả hiệu chuẩn trên file

Flow chart to calibration MQA dept

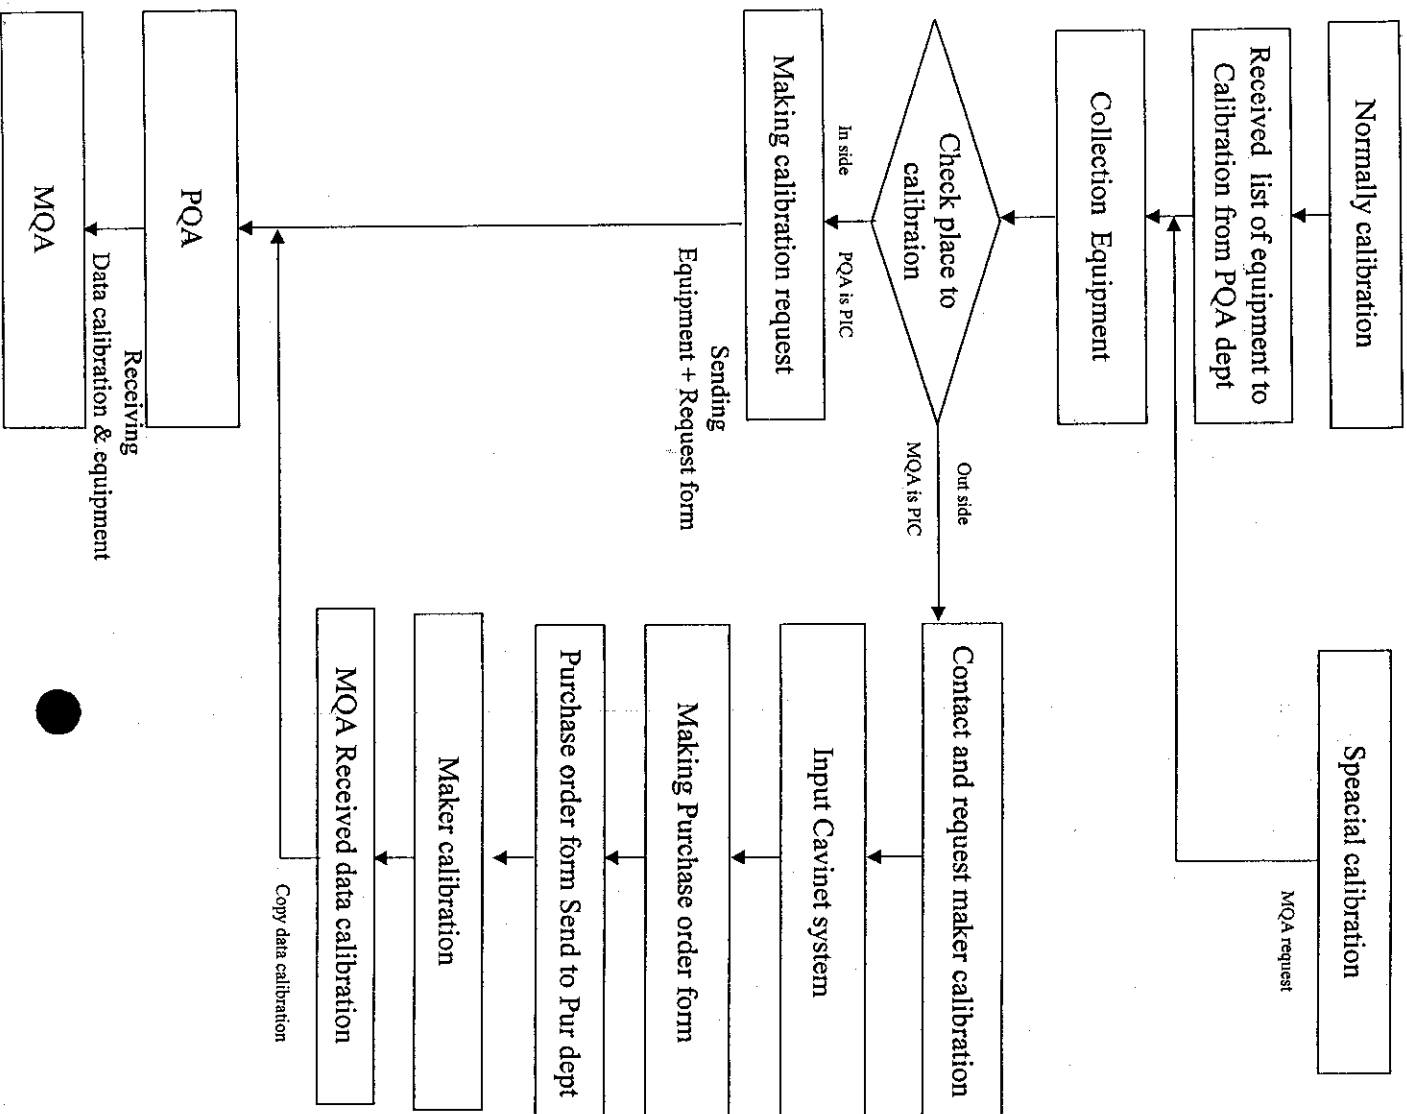

Activity content

⇒	+ List equipment received from PQA everymonth (by Email)
⇒	+ PQA member incharge : Mr Quy Anh , Mr Thai
⇒	+ P.I.C of MQA member : Mr Duy , Mr Tuan
⇒	+ MQA member send equipment to PQA before 1 day schedule
⇒	+ MQA of PIC : Ms Tuyet , Ms Luong
⇒	+ PQA of PIC : Mr Quy Anh , Mr Thai
⇒	+ Request maker send the quotation to MQA
⇒	+ Confirmation date of calibration
⇒	+ Input the calibration request into Cavinnet system
⇒	+ Print the Purchase approval sheet .Then approval by manager ,GM,FM..
⇒	+ Send the Purchase approval form to Pur dept
⇒	+ Maker go to the Canon for calibration
⇒	+ Received origin data calibration
⇒	+ Paste calibration certificated on the machine
⇒	+ Copy the data calibration to PQA (PQA of PIC: Mr Quy Anh)
⇒	+ Keeping the data calibration on file .

Ver :01

Approval by :

Issued by :


[Signature]

[Signature]

Approval	issue
<i>Commit</i>	<i>Shuby</i>

QUY TRÌNH XỬ LÝ CÁC THIẾT BỊ ĐO BỊ NG

PROCEDURE REPAIR NG EQUIPMENT

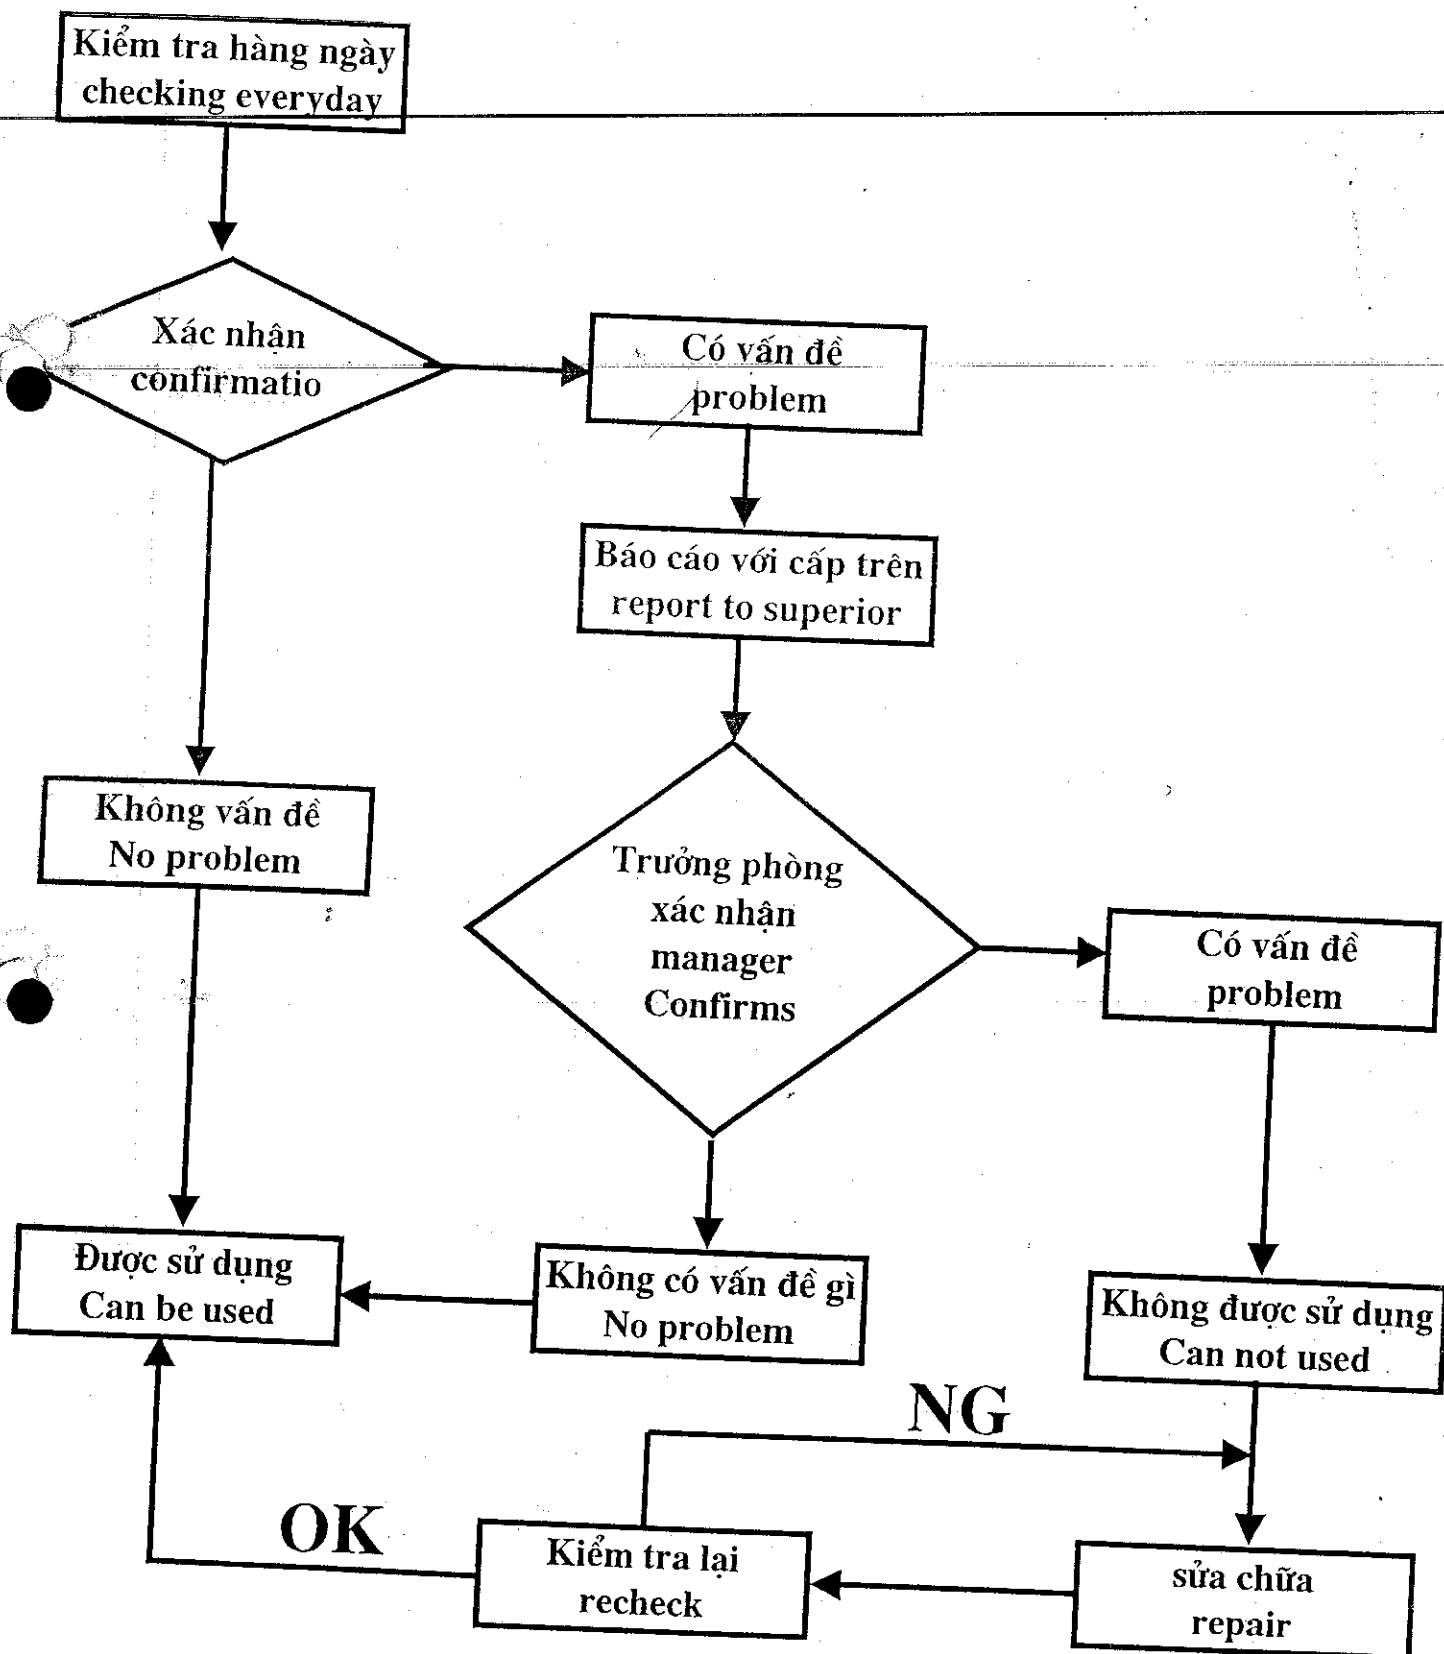

CALIBRATION REQUEST

Rev: 03 LPQA-0009-04

For request Dept.

For LPQA Dept.

+ Control No. ... 323 ...

Requested by	Dept. name	MQA		
	Requested by	Le Thi Tuyet	Phone: 9781	
Remark				
Cal. Content	☒ Periodical ☐ Special ☐ New buy ☐ Other			

Control Dept.	LPQA Dept.
Receive date	09. 01. 2010
Finish date	22. 01. 2010
Judgement	OK

+ Incase, " Control Dept" is also Department of person who request,

Department name of person who request is purned.

+ This sheet have to be enclosed with measuring equipments.

[illegible]

Issued by	CVN LBP-PQA Dept.	File No.	VLPQA001-JAN10-012	Approved by	Checked by	Written by
Model : Not classify				10. Feb 10	51 Feb 10	28. Jan 2010
REPORT ABOUT CALIBRATION RESULT IN JAN- 2010						Anh N.L.Q.Anh

1. Purpose

I would like to send to person in charges of related Division and Department about the Calibration result

2. Conclusion

According to the schedule in Jan, 2010. There are 59 measuring equipments has been calibrated. Among, Internal calibration equipments are 37 pcs and external calibration equipments are 22 pcs. However, there was 01 measuring equipment (Disk Micrometer of LMSD Dept.) already added into schedule. Therefore, there were 60 measuring equipments has been calibrated in January - 2010

The result of them are OK.


3. Calibration result

- LASSY Dept.(25pcs): 04 pcs AC Grounding Hi-testers, 04 pcs Dial Gauge Indicators, 04 pcs Digital 3154 MΩ Hi-Testers, 03 pcs Digital 3453 MΩ Hi-Testers, 04 pcs Digital 34970A Multimeters, 01 pc Digital Multimeter 8808A, 01 pc Electronic Balance and 04 pcs Withstanding Voltage Testers.
- MOLD Dept.(05pcs): 01 pc Coordinate Measuring Machine, 02 pcs Digimatic Callipers, 01 pc Outside Micrometer 01 pc Digimatic Heigh Gauge
- LMQA Dept.(18pcs): 01 pc Outside Micrometer, 03 pcs Coordinate Measuring Machines, 02 pcs Dial Tension Gauges, 01 pc Digimatic Calliper, 01 pc Digimatic Heigh Gauge, 03 pcs Disk Micrometers, 01 pc Inside Micrometer, 04 pcs Outside Micrometers and 02 pcs Spline Micrometers
- LMSD Dept.(05pcs): 01 pc Dial Test Indicator, 02 pcs Digimatic Callipers, 01 pc Outside Micrometer and 01 pc Disk Micrometer
- LPDE Dept.(02pcs): 01 pc Vernier Calliper, 01 pc Digital Multimeter.
- LPE1 Dept.(01pc): 01 pc Outside Micrometer.
- LPQA Dept. (04pcs): 02 pcs Digimatic Callipers, 01 pc Universal Power Analyzer, 01 pc Leak Current Hi-Tester

+ The calibration start date: 09. Jan. 2010

+ The calibration finish date: 26. Jan. 2010

+ Please kindly refer to attached files for more details.

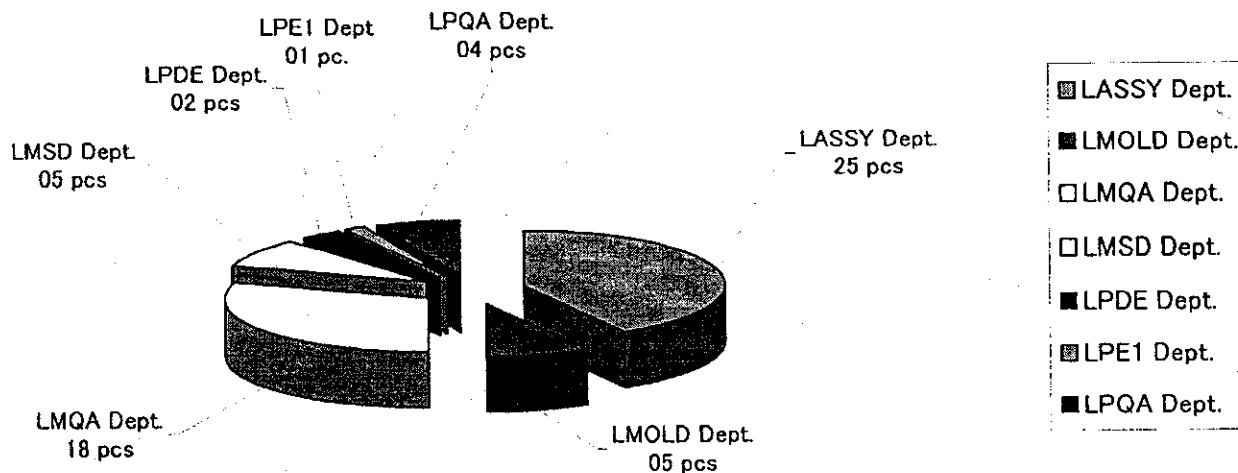

Distribute to:

Shimomaru
Susono

Toride

CVN

Other

(From Page 1 / 3 to Page 3 / 3)

- ☐ Peripherals Project Planning Div. 1 ☐ Peripherals Project Planning Dept. () ☐ Other ()
☐ Peripherals Development Center () ☐ Peripherals Design Div. () ☐ Peripherals Design Dept. ()
☐ PPQA Center ☐ PP Quality Promotion Div. () ☐ PP Quality Promotion Dept. ()
☐ PP Field Support Div. ☐ PP Field Support Dept. () ☐ Other ()
☐ PP Global Manufacturing Management Center ☐ LBP Manufacturing Engineering Div. ()
☐ LBP Manufacturing Engineering Dept. () ☐ LBP Parts Quality Assurance Dept.
☐ LBP Products Quality Assurance Div. ☐ LBP Products Quality Administration Dept.
☐ LBP Products Quality Assurance Dept. () ☐ Other ()
☐ General Director ☐ Que Vo Factory Manager ☐ LBP-PDC Div. ☐ LBP Eng. Div. ☐ LBP QA Div. ☐ LBP Manuf. Div. 1
☐ LBP Manuf. Div. 2 ☐ CRG Manuf. Div. ☐ LBP-HR&GA ☐ LBP-Plan ☐ LBP-Pur ☐ LBP-PDC ☐ Log ☐ LBP-PE1 ☐ LBP-PE2
☐ LBP-PDE ☐ LBP Parts Eng. ☐ LBP-MQA ☐ LBP-Mold ☐ LBP-MSD ☐ LBP-PCB ☐ LBP Assy management ☐ LBP-Assy1
☐ LBP-Assy2 ☐ IJ-PQA ☐ IJ-MQA ☐ Other ()
☐ Canon Zhongshan Business Machines / Product QA Div.

Measurement Equipments Calibration List

No.	Equipments name	Model no.	Maker	Serial no.	Control No.	Interval	Dept.	Cal. date	Due date	Sub-standard Measurement Equipment used	Calibrated by	Result	Remark
1	Vernier Caliper	N-15	Mitutoyo	51331764	132100900V	12	PDE	14-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
2	Digimatic High Gauge	HDM-30A	Mitutoyo	0514279	132300940V	12	MOLD	11-Jan-10	Jan-11	Height Gauge Master, Dial Test Master, Block Gauge Master	Quevo Factory member	OK	
3	Digimatic High Gauge	HDM-80A	Mitutoyo	0515468	132300990V	12	MOA	11-Jan-10	Jan-11	Height Gauge Master, Dial Test Master, Block Gauge Master	Quevo Factory member	OK	
4	Digimatic Caliper	CD-S15CT 500-454	Mitutoyo	05427830	132501050V	12	POA	14-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
5	Digimatic Caliper	CD-S15CT 500-454	Mitutoyo	05427875	132501060V	12	POA	14-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
6	Digimatic Caliper	CD-20CX 500-152-20	Mitutoyo	05237467	132501130V	12	MOA	11-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
7	Digimatic Caliper	CD-30PM	Mitutoyo	1001717	132501170V	12	MOLD	09-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
8	Digimatic Caliper	CD-45C	Mitutoyo	0011708	132501190V	12	MOLD	09-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
9	Digimatic Caliper	CD-S15CT(500-454)	Mitutoyo	05237202	132501210V	12	MSD	13-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
10	Outside Micrometer	MDCO-25MJ	Mitutoyo	55237202	133101320V	12	MOA	12-Jan-10	Jan-11	Gauge Block Set, Optical Parallel	Quevo Factory member	OK	
11	Outside Micrometer	MDC35-50MJ	Mitutoyo	45215186	133101350V	12	MOA	12-Jan-10	Jan-11	Gauge Block Set, Optical Parallel	Quevo Factory member	OK	
12	Outside Micrometer	OMP-25DM	Mitutoyo	56199805	133101390V	12	MOA	13-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
13	Spindle Micrometer	SPM3-25MJ	Mitutoyo	55183921	133101410V	12	MOA	13-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
14	Spindle Micrometer	SPM2-25MJ	Mitutoyo	55200223	133101430V	12	MOA	13-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
15	Blade Micrometer	BLM-23M	Mitutoyo	55161350	133101450V	12	MOA	11-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
16	Outside Micrometer	BTM-25	Mitutoyo	56035142	133101490V	12	MOA	12-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
17	Outside Micrometer	MDCO-25MJ	Mitutoyo	55237421	133101520V	12	MOLD	11-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
18	Inside Micrometer	IMP-30DM	Mitutoyo	55240382	133201610V	12	MOA	12-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
19	Disk Micrometer	PDM-29M	Mitutoyo	55240175	133401530V	12	MOA	12-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
20	Disk Micrometer	PDM-50M	Mitutoyo	55269407	133401550V	12	MOA	12-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
21	Disk Micrometer	PPM-25	Mitutoyo	55241580	133401570V	12	MOA	12-Jan-10	Jan-11	Gauge Block Set	Quevo Factory member	OK	
22	Disk Micrometer	GMA-25MJ(323-250)	Mitutoyo	65120820	133401590V	12	MSD	14-Jan-10	Jan-11	Gauge Block Set, Optical Parallel	Quevo Factory member	OK	It was added into schedule
23	Dial Gauge Indicator	1044FB-10	Mitutoyo	1044FB-10	134101970V	12	ASSY	09-Jan-10	Jan-11	Calibration Tester	Quevo Factory member	OK	
24	Dial Gauge Indicator	1044FB-10	Mitutoyo	1044FB-10	134101980V	12	ASSY	09-Jan-10	Jan-11	Calibration Tester	Quevo Factory member	OK	
25	Dial Gauge Indicator	1044FB-10	Mitutoyo	1044FB-10	134101990V	12	ASSY	09-Jan-10	Jan-11	Calibration Tester	Quevo Factory member	OK	
26	Dial Gauge Indicator	1044FB-10	Mitutoyo	1044FB-10	134102000V	12	ASSY	09-Jan-10	Jan-11	Calibration Tester	Quevo Factory member	OK	
27	Dial Test Indicator	TI-1235(13-415S)	Mitutoyo	FVE726	134202330V	12	MSD	13-Jan-10	Jan-11	Calibration Tester	Quevo Factory member	OK	
28	Coordinate Measuring Machine	CVA1010A	Accretach	GB6551M2	151302400V	12	MOA	13-Jan-10	Jan-11	Gauge Block Set	Tokyo Seimitsu	OK	
29	Coordinate Measuring Machine	CVA1012A	Accretach	GB6751AA	151302410V	12	MOLD	11-Jan-10	Jan-11	Gauge Block Set	Tokyo Seimitsu	OK	
30	Coordinate Measuring Machine	AE122	Mitutoyo	88021039	151302420V	12	MOA	19-Jan-10	Jan-11	Gauge Block Set	Tokyo Seimitsu	OK	
31	Coordinate Measuring Machine	CVA1010A	Accretach	GB6551MA	151302430V	12	MOA	11-Jan-10	Jan-11	Gauge Block Set	Tokyo Seimitsu	OK	
32	Digimatic Caliper	CD-80C 500-501-10	Mitutoyo	0019590	132502930V	12	MSD	13-Jan-10	Jan-11	Caliper checker	Quevo Factory member	OK	
33	Outside Micrometer	M110-25	Mitutoyo	85462445	133104090V	12	MSD	14-Jan-10	Jan-11	Gauge Block Set, Optical Parallel	Quevo Factory member	OK	
34	Outside Micrometer	MDC-25MJ T	Mitutoyo	45081511	133104100V	12	PEI	14-Jan-10	Jan-11	Gauge Block Set, Optical Parallel	Quevo Factory member	OK	
35	Dial Tension Gauge	50mN	Mitutoyo	315088	221300330V	12	MOA	11-Jan-10	Jan-11	Weight Standard	Quevo Factory member	OK	
36	Dial Tension Gauge	50mN	Mitutoyo	315081	221300340V	12	MOA	11-Jan-10	Jan-11	Weight Standard	Quevo Factory member	OK	
37	Electronic Balance	BL-220H W/AC	Shimadzu	043205255	212401170V	12	ASSY	09-Jan-10	Jan-11	Weight Standard	Quevo Factory member	OK	
38	Withstanding Voltage Tester	AC3158	Hoki	061199784	24900210V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
39	Withstanding Voltage Tester	TOS5050A	Kikusui	LF002837	20240V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	

Measurement Equipments Calibration List

No.	Equipments name	Model no.	Maker	Serial no.	Control No.	Interval	Dept.	Cal. date	Due date	Sub-standard Measurement Equipment used	Calibrated by	Result	Remark
40	Withstanding Voltage Tester	AC3158	Hoki	070399385	311900280V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
41	Digital 3154 MQ H-T-Tester	3154	Hoki	070134204	312601370V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
42	Digital 3154 MQ H-T-Tester	3154	Hoki	070206425	312601470V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
43	Digital 3154 MQ H-T-Tester	3154	Hoki	070206426	312601480V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
44	Digital 34970A Multimeter	34970A	Agilent	MV44022628	312601500V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
45	Digital 34970A Multimeter	34970A	Agilent	MV44021977	312601560V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
46	Digital 3154 MQ H-T-Tester	3154	Hoki	060228515	312602200V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
47	Digital 34970A Multimeter	34970A	Agilent	MV44029377	312602330V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
48	Digital 34970A Multimeter	34970A	Agilent	MV44029311	312602590V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
49	AC Grounding HI-Tester	3157	Hoki	060218578	318702950V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
50	AC Grounding HI-Tester	3157	Hoki	070123439	318703040V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
51	AC Grounding HI-Tester	3157	Hoki	070118891	318703050V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
52	AC Grounding HI-Tester	3157	Hoki	070136255	318703060V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
53	Digital Multimeter	177 True RMS	Fuke	89730058	312603720V	12	POE	14-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Queva Factory member	OK	
54	Withstanding Voltage Tester	AC3158	Hoki	070399388	311903860V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
55	Digital 3453 MQ H-T-Tester	3453	Hoki	051018481	312603900V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
56	Digital 3453 MQ H-T-Tester	3453	Hoki	070209970	312603980V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
57	Digital 3453 MQ H-T-Tester	3453	Hoki	070335620	312603990V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
58	Universal Power Analyzer	PM6000	VOLTECH	20006700278	318904870V	12	POA	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
59	Leak Current HI-Tester	3156	HIOKI	80806856	311904880V	12	POA	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	
60	Digital Multimeter 8808A	8808A	Fuke	9557006	312604960V	12	ASSY	12-Jan-10	Jan-11	Refer to Certificate of Nihon Denkei VN Co., Ltd	Nihon Denkei VN Co., Ltd	OK	

THE REGISTER OF MEASURING EQUIPMENTS CALIBRATION -2010

Ver :01

Approval by :

Issued by :

LBP-MQA Department *Phang Jau*

No.	Measuring Equipment Name	Maker	Control No.	Interval	Cal. Date	Due	Status	Cal place	Monthly checking		Remark
									Result	Date	
1	Hardness machine	MTT - X7	MM5278X	24	22-Dec-09	22-Dec-11	On use	Outside			
2	Gauge Block Set	Multibo	12310001QV	36	16-Dec-08	Nov-11	On use	Outside			
3	Pin Gauge	Eisen	12920051QV	36	13-Nov-08	Nov-11	On use	Inhouse			
4	Pin Gauge	Eisen	12920052QV	36	14-Nov-08	Nov-11	On use	Inhouse			
5	Pin Gauge	Eisen	12920053QV	36	14-Nov-08	Nov-11	On use	Inhouse			
6	Pin Gauge	Eisen	12920054QV	36	15-Nov-08	Nov-11	On use	Inhouse			
7	Pin Gauge	Eisen	12920055QV	36	15-Nov-08	Nov-11	On use	Inhouse			
8	Pin Gauge	Eisen	12920056QV	36	17-Nov-08	Nov-11	On use	Inhouse			
9	Pin Gauge	Eisen	12920057QV	36	17-Nov-08	Nov-11	On use	Inhouse			
10	Pin Gauge	Eisen	12920058QV	36	18-Nov-08	Nov-11	On use	Inhouse			
11	Pin Gauge	Eisen	12920059QV	36	18-Nov-08	Nov-11	On use	Inhouse			
12	Pin Gauge	Eisen	12920060QV	36	19-Nov-08	Nov-11	On use	Inhouse			
13	Pin Gauge	Eisen	12920061QV	36	19-Nov-08	Nov-11	On use	Inhouse			
14	Pin Gauge	Eisen	12920062QV	36	20-Nov-08	Nov-11	On use	Inhouse			
15	Pin Gauge	Eisen	12920063QV	36	20-Nov-08	Nov-11	On use	Inhouse			
16	Pin Gauge	Eisen	12920038QV	36	10-Oct-08	Oct-11	On use	Inhouse			
17	Pin Gauge	Eisen	12920039QV	36	13-Oct-08	Oct-11	On use	Inhouse			
18	Pin Gauge	Eisen	12920040QV	36	13-Oct-08	Oct-11	On use	Inhouse			
19	Pin Gauge	Eisen	12920041QV	36	14-Oct-08	Oct-11	On use	Inhouse			
20	Pin Gauge	Eisen	12920042QV	36	14-Oct-08	Oct-11	On use	Inhouse			
21	Pin Gauge	Eisen	12920043QV	36	15-Oct-08	Oct-11	On use	Inhouse			
22	Pin Gauge	Eisen	12920044QV	36	15-Oct-08	Oct-11	On use	Inhouse			
23	Pin Gauge	Eisen	12920045QV	36	16-Oct-08	Oct-11	On use	Inhouse			

Measuring Equipment Name	Maker	Control No.	Interval	Cal. Date	Due	Status	Cal place	Monthly checking		Remark
								Result	Date	
24 Pin Gauge	Eisen	12920046QV	36	16-Oct-08	Oct-11	On use	Inhouse			
25 Pin Gauge	Eisen	12920047QV	36	17-Oct-08	Oct-11	On use	Inhouse			
26 Pin Gauge	Eisen	12920048QV	36	17-Oct-08	Oct-11	On use	Inhouse			
27 Pin Gauge	Eisen	12920049QV	36	20-Oct-08	Oct-11	On use	Inhouse			
28 Pin Gauge	Eisen	12920050QV	36	20-Oct-08	Oct-11	On use	Inhouse			
29 Pin Gauge	Eisen	12920026QV	36	12-Sep-08	Sep-11	On use	Inhouse			
30 Pin Gauge	Eisen	12920027QV	36	15-Sep-08	Sep-11	On use	Inhouse			
31 Pin Gauge	Eisen	12920028QV	36	15-Sep-08	Sep-11	On use	Inhouse			
32 Pin Gauge	Eisen	12920029QV	36	16-Sep-08	Sep-11	On use	Inhouse			
33 Pin Gauge	Eisen	12920030QV	36	16-Sep-08	Sep-11	On use	Inhouse			
34 Pin Gauge	Eisen	12920031QV	36	17-Sep-08	Sep-11	On use	Inhouse			
35 Pin Gauge	Eisen	12920032QV	36	17-Sep-08	Sep-11	On use	Inhouse			
36 Pin Gauge	Eisen	12920033QV	36	18-Sep-08	Sep-11	On use	Inhouse			
37 Pin Gauge	Eisen	12920034QV	36	18-Sep-08	Sep-11	On use	Inhouse			
38 Pin Gauge	Eisen	12920035QV	36	19-Sep-08	Sep-11	On use	Inhouse			
39 Pin Gauge	Eisen	12920036QV	36	19-Sep-08	Sep-11	On use	Inhouse			
40 Pin Gauge	Eisen	12920037QV	36	19-Sep-08	Sep-11	On use	Inhouse			
41 Granite Surface Plate	Mitutoyo	12990080QV	36	24-Sep-08	Sep-11	On use	Outside			
42 Granite Surface Plate	MSK	12990081QV	36	24-Sep-08	Sep-11	On use	Outside			
43 Push-Pull Gauge	Imada	22160043QV	24	15-Sep-09	Sep-11	On use	Inhouse			
44 Push-Pull Gauge	Imada	22160044QV	24	15-Sep-09	Sep-11	On use	Inhouse			
45 Push-Pull Gauge	Imada	22160042QV	24	19-Aug-09	Aug-11	On use	Inhouse			
46 Push-Pull Gauge	Imada	22160040QV	24	14-Jul-09	Jul-11	On use	Inhouse			
47 Push-Pull Gauge	Imada	22160041QV	24	15-Jul-09	Jul-11	On use	Inhouse			
48 Wrist Strap Tester	3M	37980354QV	24	15-Jul-09	Jul-11	On use	Inhouse			
49 Flooring Tester	3M	37980356QV	24	11-Jun-09	Jun-11	On use	Inhouse			
50 X-Ray Machine 1200VX	QES	69990006	12	17-Dec-09	17-Dec-10	On use	Outside			

Measuring Equipment Name	Maker	Control No.	Interval	Cal. Date	Due	Status	Cal place	Monthly checking		Remark
								Result	Date	
51 Digimatic Height Gauge	Mitutoyo	13230092QV	12	16-Dec-09	Dec-10	On use	Inhouse			
52 Digimatic Calliper	Mitutoyo	13250109QV	12	16-Dec-09	Dec-10	On use	Inhouse			
53 Outside Micrometer	Mitutoyo	13310128QV	12	17-Dec-09	Dec-10	On use	Inhouse			
54 Outside Micrometer	Mitutoyo	13310129QV	12	17-Dec-09	Dec-10	On use	Inhouse			
55 Outside Micrometer	Mitutoyo	13310130QV	12	17-Dec-09	Dec-10	On use	Inhouse			
56 Outside Micrometer	Mitutoyo	13310131QV	12	17-Dec-09	Dec-10	On use	Inhouse			
57 Outside Micrometer	Mitutoyo	13310134QV	12	17-Dec-09	Dec-10	On use	Inhouse			
58 Outside Micrometer	Mitutoyo	13310136QV	12	17-Dec-09	Dec-10	On use	Inhouse			
59 Outside Micrometer	Mitutoyo	13310137QV	12	17-Dec-09	Dec-10	On use	Inhouse			
60 Outside Micrometer	Mitutoyo	13310138QV	12	17-Dec-08	Dec-10	On use	Inhouse			
61 Spline Micrometer	Mitutoyo	13310140QV	12	18-Dec-09	Dec-10	On use	Inhouse			
62 Spline Micrometer	Mitutoyo	13310142QV	12	18-Dec-09	Dec-10	On use	Inhouse			
63 Blade Micrometer	Mitutoyo	13310144QV	12	16-Dec-09	Dec-10	On use	Inhouse			
64 Outside Micrometer	Mitutoyo	13310146QV	12	16-Dec-09	Dec-10	On use	Inhouse			
65 Outside Micrometer	Mitutoyo	13310147QV	12	16-Dec-09	Dec-10	On use	Inhouse			
66 Disk Micrometer	Mitutoyo	13340162QV	12	16-Dec-09	Dec-10	On use	Inhouse			
67 Disk Micrometer	Mitutoyo	13340166QV	12	16-Dec-09	Dec-10	On use	Inhouse			
68 Electronic Balance	A&D	21240090QV	12	17-Nov-09	Nov-10	On use	Inhouse			
69 HI Tester	Hioki	31260090QV	12	18-Nov-09	Nov-10	On use	Inhouse			
70 LCR Tester	Hioki	34420347QV	24	11-Nov-08	Nov-10	On use	Outside			
71 CMM Gear Machine	Osaka Seimitsu Kikai	17910389QV	12	28-Oct-09	28-Oct-10	On use	Outside			
72 Gear Rolling Tester	Osaka Seimitsu Kikai	17910401QV	12	28-Oct-09	28-Oct-10	On use	Outside			
73 Digimatic Calliper	Mitutoyo	13250108QV	12	14-Oct-09	Oct-10	On use	Inhouse			
74 Digimatic Calliper	Mitutoyo	13250125QV	12	14-Oct-09	Oct-10	On use	Inhouse			
75 Disk Micrometer	Mitutoyo	13340164QV	12	14-Oct-09	Oct-10	On use	Inhouse			
76 Dial Test Indicator	Mitutoyo	13420232QV	12	14-Oct-09	Oct-10	On use	Inhouse			
77 Electronic Balance	A&D	21240080QV	12	14-Oct-09	Oct-10	On use	Inhouse			

Measuring Equipment Name	Maker	Control No.	Interval	Cal. Date	Due	Status	Cal place	Monthly checking		Remark
								Result	Date	
78 HI_Tester	Hioki	31260091QV	12	15-Oct-09	Oct-10	On use	Inhouse			
79 X-Ray Machine 6000 VX	OES		12	8-Sep-09	8-Sep-10	On use	Outside			
80 Dial Test Indicator	Mitutoyo	13420229QV	12	15-Sep-09	Sep-10	On use	Inhouse			
81 Dial Test Indicator	Mitutoyo	13420230QV	12	15-Sep-09	Sep-10	On use	Inhouse			
82 Measuring Microscope	Nikon	15220400QV	12	18-Sep-09	Sep-10	On use	Outside			
83 HI_Tester	Hioki	31260088QV	12	15-Sep-09	Sep-10	On use	Inhouse			
84 HI_Tester	Hioki	31260089QV	12	15-Sep-09	Sep-10	On use	Inhouse			
85 Twist coil spring testing machine	STM Mfg Co.Ltd	22910046QV	12	31-Aug-09	31-Aug-10	On use	Inhouse			
86 Twist coil spring testing machine	STM Mfg Co.Ltd	22910047QV	12	31-Aug-09	31-Aug-10	On use	Inhouse			
87 Digimatic Height Gauge	Mitutoyo	13230098QV	12	18-Aug-09	Aug-10	On use	Inhouse			
88 Digimatic Height Gauge	Mitutoyo	13230100QV	12	18-Aug-09	Aug-10	On use	Inhouse			
89 HI_Tester	Hioki	31260087QV	12	19-Aug-09	Aug-10	On use	Inhouse			
90 Digimatic Height Gauge	Mitutoyo	13230096QV	12	14-Jul-09	Jul-10	On use	Inhouse			
91 Digimatic Height Gauge	Mitutoyo	13230097QV	12	15-Jul-09	Jul-10	On use	Inhouse			
92 Torque Driver	Tohnichi	23110061QV	12	15-Jul-09	Jul-10	On use	Inhouse			
93 Vernier Calliper	Mitutoyo	13210088QV	12	12-Jun-09	Jun-10	On use	Inhouse			
94 Dial Test Indicator	Mitutoyo	13420227QV	12	11-Jun-09	Jun-10	On use	Inhouse			
95 Dial Test Indicator	Mitutoyo	13420228QV	12	11-Jun-09	Jun-10	On use	Inhouse			
96 Torque Driver	Tohnichi	23110055QV	12	11-Jun-09	Jun-10	On use	Inhouse			
97 Torque Driver	Tohnichi	23110059QV	12	11-Jun-09	Jun-10	On use	Inhouse			
98 Torque Driver	Tohnichi	23110060QV	12	12-Jun-09	Jun-10	On use	Inhouse			
99 Digital 34401A Multimeter	Agilent	31260075QV	12	11-Jun-09	Jun-10	On use	Outside			
100 Vernier Calliper	Mitutoyo	13210083QV	12	20-May-09	May-10	On use	Inhouse			
101 Vernier Calliper	Mitutoyo	13210085QV	12	20-May-09	May-10	On use	Inhouse			
102 Digimatic Calliper	Mitutoyo	13250112QV	12	19-May-09	May-10	On use	Inhouse			
103 Dial Test Indicator	Mitutoyo	13420225QV	12	18-May-09	May-10	On use	Inhouse			
104 Dial Test Indicator	Mitutoyo	13420222	12	18-May-09	May-10	On	Inhouse			

Measuring Equipment Name	Maker	Control No.	Interval	Cal. Date	Due	Status	Cal place	Monthly checking		Remark
								Result	Date	
105 Digimatic Calliper	Mitutoyo	13250287QV	12	19-May-09	May-10	On use	Inhouse			
106 Digimatic Calliper	Mitutoyo	13250288QV	12	19-May-09	May-10	On use	Inhouse			
107 Torque Driver	Tohnichi	23110053QV	12	19-May-09	May-10	On use	Inhouse			
108 Torque Driver	Tohnichi	23110054QV	12	19-May-09	May-10	On use	Inhouse			
109 Torque Driver	Tohnichi	23110056QV	12	19-May-09	May-10	On use	Inhouse			
110 Torque Driver	Tohnichi	23110057QV	12	20-May-09	May-10	On use	Inhouse			
111 Torque Driver	Tohnichi	23110058QV	12	20-May-09	May-10	On use	Inhouse			
112 Thickness Gauge(25 leaf)	TSK	12320004QV	24	18-Apr-08	Apr-10	On use	Inhouse			
113 Thickness Gauge(25 leaf)	TSK	12320005QV	24	19-Apr-08	Apr-10	On use	Inhouse			
114 Thickness Gauge(25 leaf)	TSK	12320022QV	24	19-Apr-08	Apr-10	On use	Inhouse			
115 Thickness Gauge(25 leaf)	TSK	12320023QV	24	19-Apr-08	Apr-10	On use	Inhouse			
116 Thickness Gauge(25 leaf)	TSK	12320024QV	24	19-Apr-08	Apr-10	On use	Inhouse			
117 Thickness Gauge(25 leaf)	TSK	12320025QV	24	19-Apr-08	Apr-10	On use	Inhouse			
118 Vernier Calliper	Mitutoyo	13210087QV	12	20-Apr-09	Apr-10	On use	Inhouse			
119 Vernier Calliper	Mitutoyo	13210091QV	12	20-Apr-09	Apr-10	On use	Inhouse			
120 Digimatic Calliper	Mitutoyo	13250110QV	12	17-Apr-09	Apr-10	On use	Inhouse			
121 Digimatic Calliper	Mitutoyo	13250114QV	12	17-Apr-09	Apr-10	On use	Inhouse			
122 Outside Micrometer	Mitutoyo	13310156QV	12	17-Apr-09	Apr-10	On use	Inhouse			
123 Outside Micrometer	Mitutoyo	13310157QV	12	20-Apr-09	Apr-10	On use	Inhouse			
124 Spine Micrometer	Mitutoyo	13310158QV	12	20-Apr-09	Apr-10	On use	Inhouse			
125 Laser Micro Gauge	TOE	17910402QV	24	7-May-08	May-10	On use	Outside			
126 Vernier Calliper	Mitutoyo	13210084QV	12	17-Mar-09	Mar-10	On use	Inhouse			
127 Digimatic Calliper	Mitutoyo	13250111QV	12	16-Mar-09	Mar-10	On use	Inhouse			
128 Digimatic Calliper	Mitutoyo	13250126QV	12	16-Mar-09	Mar-10	On use	Inhouse			
129 Outside Micrometer	Mitutoyo	13310133QV	12	17-Mar-09	Mar-10	On use	Inhouse			
130 Outside Micrometer	Mitutoyo	13310148QV	12	17-Mar-09	Mar-10	On use	Inhouse			
132 Disk Micrometer	Mitutoyo	13340168QV	12	17-Mar-09	Mar-10	On use	Inhouse			

Measuring Equipment Name	Maker	Control No.	Interval	Cal. Date	Due	Status	Cal place	Monthly checking		Remark
								Result	Date	
133 Digital Magnet scale	Mitutoyo	15120238QV	12	17-Mar-09	Mar-10	On use	Inhouse	OK	29/Jan	
134 Digimatic Height Gauge	Mitutoyo	13230099QV	12	11-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
135 Digimatic Caliper	Mitutoyo	13250113QV	12	11-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
136 Outside Micrometer	Mitutoyo	13310132QV	12	12-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
137 Outside Micrometer	Mitutoyo	13310135QV	12	12-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
138 Outside Micrometer	Mitutoyo	13310139QV	12	13-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
139 Spline Micrometer	Mitutoyo	13310141QV	12	13-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
140 Spline Micrometer	Mitutoyo	13310143QV	12	13-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
141 Blade Micrometer	Mitutoyo	13310145QV	12	11-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
142 Outside Micrometer	Mitutoyo	13310149QV	12	12-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
143 Inside Micrometer	Mitutoyo	13320161QV	12	12-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
144 Disk Micrometer	Mitutoyo	13340163QV	12	12-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
145 Disk Micrometer	Mitutoyo	13340165QV	12	12-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
146 Disk Micrometer	Mitutoyo	13340167QV	12	12-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
147 Coordinate Measuring Machine	Accretech	15130240QV	12	13-Jan-09	Jan-10	On use	Outside	OK	29/Jan	
148 Coordinate Measuring Machine	Mitutoyo	15130242QV	12	19-Jan-09	Jan-10	On use	Outside	OK	29/Jan	
149 Coordinate Measuring Machine	Accretech	15130243QV	12	11-Jan-09	Jan-10	On use	Outside	OK	29/Jan	
150 Dial Tension Gauge	Mitutoyo	22130033QV	12	11-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
151 Dial Tension Gauge	Mitutoyo	22130034QV	12	11-Jan-09	Jan-10	On use	Inhouse	OK	29/Jan	
131 Outside Micrometer	Mitutoyo	13310159QV	12	17-Mar-09	Mar-10	Storage				
152 Spline Micrometer	Mitutoyo	13310201QV	12	1-Oct-07	Oct-08	Storage				
153 Disk Micrometer	Mitutoyo	13340317QV	12	1-Oct-07	Oct-08	Storage				
154 Thickness Gauge(25 leaf)	TSK	12320247QV	24	Apr-06	Apr-08	Storage				
155 Thickness Gauge(25 leaf)	TSK	12320248QV	24	Apr-06	Apr-08	Storage				
156 Thickness Gauge(25 leaf)	TSK	12320249QV	24	Apr-06	Apr-08	Storage				
158 Outside Micrometer	Mitutoyo	13310286QV	12	11-Dec-06	Dec-07	Storage				
159 Outside Micrometer	Mitutoyo	13310287QV	12	11-Dec-06	Dec-07	Storage				
160 Outside Micrometer	Mitutoyo	13310288QV	12	11-Dec-06	Dec-07	Storage				

Measuring Equipment Name	Maker	Control No.	Interval	Cal. Date	Due	Status	Cal place	Monthly checking		Remark
								Result	Date	
161	Outside Micrometer	Mitutoyo	13310289QV	12	11-Dec-06	Dec-07	Storage			
162	Outside Micrometer	Mitutoyo	13310300QV	12	12-Dec-06	Dec-07	Storage			
163	Spline Micrometer	Mitutoyo	13310302QV	12	13-Dec-06	Dec-07	Storage			
164	Spline Micrometer	Mitutoyo	13310303QV	12	13-Dec-06	Dec-07	Storage			
165	Blade Micrometer	Mitutoyo	13310304QV	12	13-Dec-06	Dec-07	Storage			
166	Outside Micrometer	Mitutoyo	13310305QV	12	13-Dec-06	Dec-07	Storage			
167	Oscilloscope	Tektronix	37310383QV	24	Nov-05(Certificate)	Nov-07	Storage			
168	Withstanding Voltage Tester	Kikusui	31190362QV	12	19-Sep-06	Sep-07	Storage			
169	DC Power Supply	Kikusui	31190369QV	24	Sep-05(Certificate)	Sep-07	Storage			
170	DC Power Supply	Kikusui	31190370QV	24	Sep-05(Certificate)	Sep-07	Storage			
171	DC Power Supply	Kikusui	31190371QV	24	Sep-05(Certificate)	Sep-07	Storage			
172	Digital 3154 MΩ HI-Tester	HioKI	31260374QV	12	19-Sep-06	Sep-07	Storage			
173	Electrostatic Field Meter	SSD	31290378QV	12	19-Sep-06	Sep-07	Storage			
174	High Voltage Probe	Tektronix	31870381QV	24	Sep-05(Certificate)	Sep-07	Storage			
175	Current Probe	Tektronix	31870380QV	24	Aug-05(Certificate)	Aug-07	Storage			
176	Automatic Roller Measurement Machine	Advantech	15230388QV	Non Cal	7-May-08	Non Cal	On use			
177	Constant Loader For Durometer	ASKER	24150127QV	Non Cal	Ap-06	Non Cal	On use			
178	X-Ray Machine NITON X1797	Regaku	69990003QV	None cal	None cal	None cal	On use			

10 / 10