

Sample ID:DT13_LCNeg5

Sample Scans:32 Background Scans:32

Resolution:4 System Status:Good

04T16-10-15.a2r

Method

Name:C:\Users\Public\Documents\Agilent\MicroLa


b\Methods\Basic IR.a2m User:Generic User

Date/Time:06/04/2019 4:10:15 PM

Range:4000 - 650

Apodization: Happ-Genzel

File Location:C:\Users\Public\Documents\Agilent\MicroLab\Results\\Basic IR\DT13_LCNeg5_2019-06-

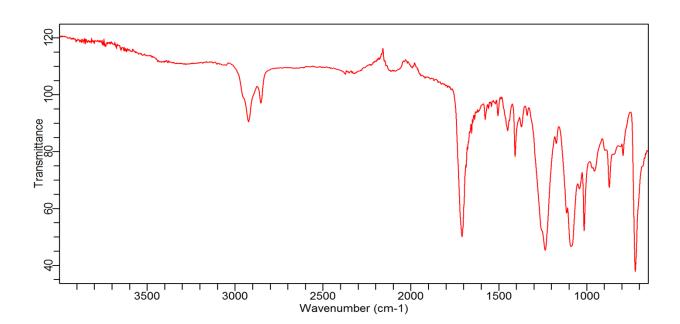

6/4/2019 4:11:32 PM page 1 of 1