

IVF Equipment Utilization Dashboard (2-Year Analysis)

total_cases_day_lab
88,639

avg_delay_minutes
149,604.3

technical_downtime_hrs
658.8

idle_hrs
62,194.75

Select date range


equipment_id

	equipment_id	total...
1.	MIC_X1	12,738
2.	INC_A2	12,726
3.	INC_A1	12,665
4.	ICSI_01	12,704
5.	MIC_X2	12,695
6.	INC_B1	12,563
7.	ICSI_02	12,548


1 - 7 / 7




TOTAL CASES BY LAB ID

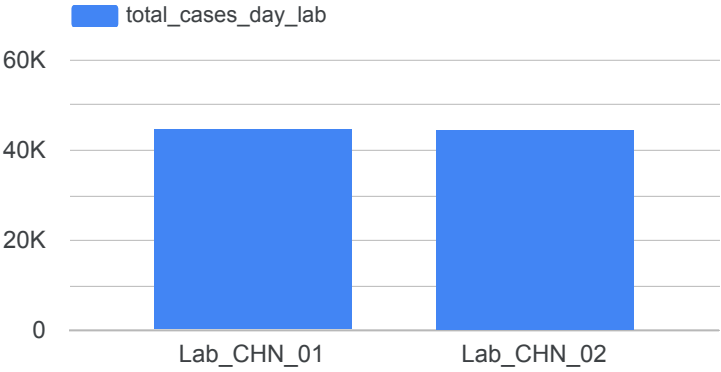

EQUIPMENT TYPE BY MANUFACTURE

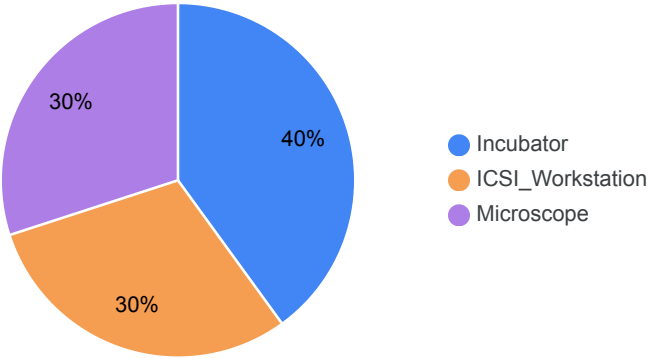

MAX CAPACITY HRS BY EQUIPMENT TYPE

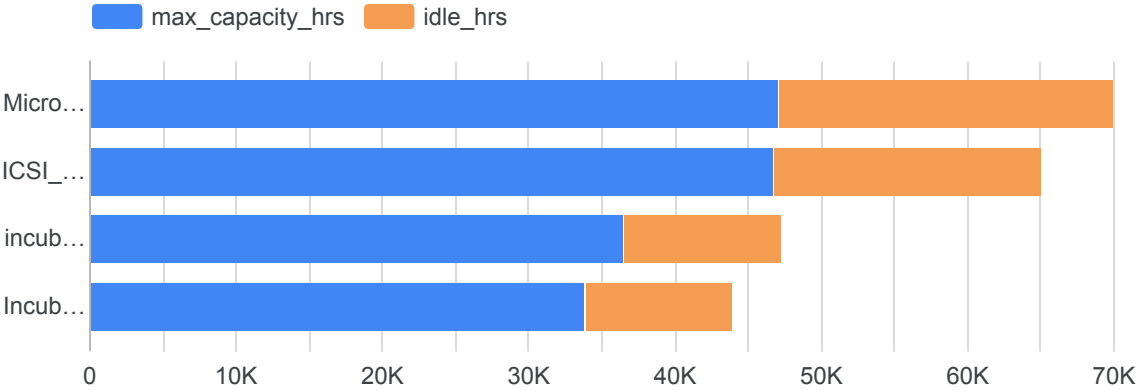

TOTAL CASES OVER TIME

