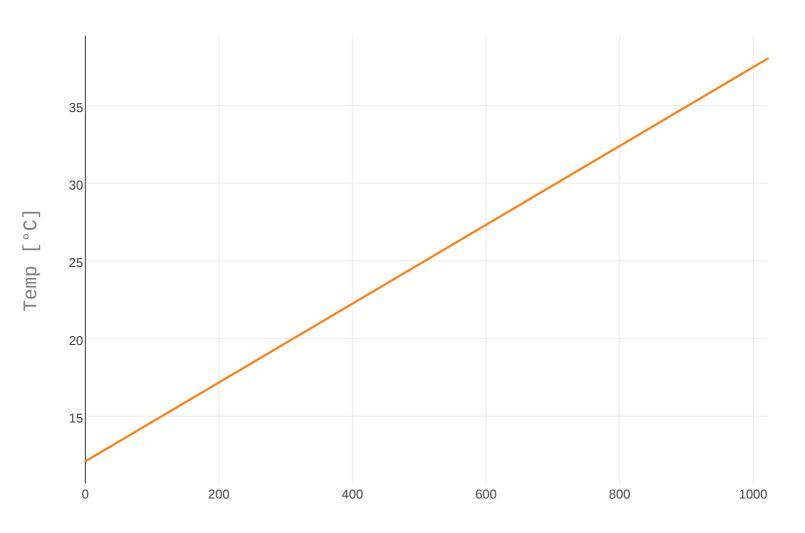Temperature calibration