

Procesamiento de imágenes médicas para el diagnóstico


Doppler response Laboratory

Andrea Corrales Romero A00828752

Tecnológico de Monterrey, Campus Monterrey

19/05/2022

1. Range-Doppler response using matched filter.

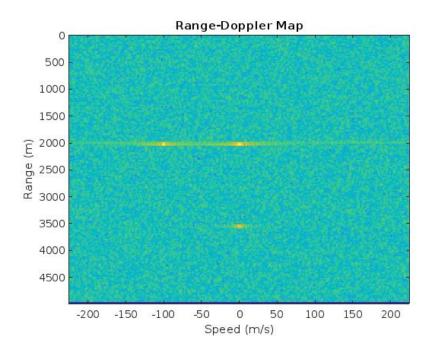

${\bf 2.} \quad {\bf Estimate\ Doppler\ and\ range\ from\ range\ Doppler\ response.}$

"The target is approximately 2250 meters away and is moving fast enough to cause a Doppler shift of approximately 712.8906 Hz."

dop_est= -712.8906 rng_est= 2250

3. Range Doppler Response of FMCW signal.

