

[Re] Optimization of a free water elimination two-compartment model for diffusion tensor imaging.

Rafael Neto Henriques¹, Ariel Rokem², Eleftherios Garyfallidis³, Samuel St-Jean⁴, Eric Thomas Peterson⁵, and Marta Morgado Correia¹

1 MRC Cognition and Brain Sciences Unit, Cambridge, Cambridgeshire, UK **2** The University of Washington eScience Institute, Seattle, WA, USA **3** Intelligent Systems Engineering, Indiana University, IA, USA **4** University Medical Center Utrecht, Utrecht, NL **5** Biosciences, SRI International, Menlo Park, CA, USA

rafaelnh21@gmail.com

Editor

Name Surname

Reviewers

Name Surname

Name Surname

Received Sep, 1, 2015

Accepted Sep, 1, 2015

Published Sep, 1, 2015

Licence [CC-BY](#)

Competing Interests:

The authors have declared that no competing interests exist.

 [Article repository](#)

 [Code repository](#)

A reference implementation of

→ Hoy, A.R., Koay, C.G., Kecskemeti, S.R., Alexander, A.L. (2014). Optimization of a free water elimination two-compartment model for diffusion tensor imaging. *NeuroImage* 103, 323-333. doi: 10.1016/j.neuroimage.2014.09.053

Introduction

Diffusion-weighted Magnetic Resonance Imaging (DW-MRI) is a biomedical imaging technique that allows for the non-invasive acquisition of *in vivo* data from which tissue microstructure can be inferred. Diffusion tensor imaging (DTI), one of the most commonly used DW-MRI techniques in the brain, models diffusion anisotropy of tissues using a second-order tensor known as the diffusion tensor (DT) [1], [2].

DTI-based measures such as fractional anisotropy (FA) and mean diffusivity (MD) are usually used to assess properties of brain microstructure. For example, FA is sensitive to different microstructural properties (such as packing density of axons, and density of myelin in nerve fibers [3]), as well to the degree of white matter coherence (i.e. the alignment of axons within a measurement voxel). However, because a measurement voxel can contain partial volumes of different types of tissue, these measures are not always specific to one particular type of tissue. In particular, diffusion anisotropy in voxels near cerebral ventricles and parenchyma can be underestimated by partial volume effects of cerebrospinal fluid (CSF).

Since CSF partial volume effects depend on the exact positioning of brain relative to the MRI spatial encoding grid, the reproducibility of diffusion-weighted measures might be compromised by free water diffusion partial volume effects [8]. Moreover, free water contaminations are likely to confound diffusion based measures in studies of brain aging and some pathology, because CSF partial volume effects might be increased due to tissue morphological atrophy and enlargement of cerebral ventricle [9].

During the MRI acquisition, the signal from free water can be directly eliminated using fluid-attenuated inversion recovery diffusion-weighted sequence [10]. However, these sequences have some drawback. For example, they require longer acquisitions times and produce images with lower SNR. Moreover, these approaches cannot be used retrospectively for data cohorts already acquired with more conventional diffusion-weighted sequences.

Diffusion free-water can also be suppressed by adding parameters to the diffusion MRI models. For example, the DTI model can be extended to separately take into account the contributions of tissue and CSF by representing the tissue compartment with an anisotropic diffusion tensor and the CSF compartment as an isotropic free water diffusion coefficient [11]. Recently, two procedures were proposed by Hoy and colleagues to fit this two compartments model to diffusion-weighted data at different b-values (i.e. different diffusion gradient-weightings) [5]. Although these procedures have been shown to provide diffusion based measures that are stable to different degrees of free water contamination, the authors noted that their original algorithms were “implemented by a group member with no formal programming training and without optimization for speed” [5].

In this work, we provide the first open-source reference implementation of the free water contamination DTI model. All implementations are made in Python for its compatibility with the previously optimized functions freely available at the software package Diffusion Imaging in Python (Dipy, [4]). In addition to some methodological improvements done to increase the model fitting robustness, here the fitting evaluation previously performed by Hoy et al. (2014) is also replicated [5]. Finally, the optimal acquisition parameter sets for fitting the free water elimination DTI model is re-accessed.

Methods

The free water elimination DTI (fwDTI) model describes the measured diffusion-weighted signal s_i with a simple bi-exponential expansion of DTI:

$$s_i = s_0 [f \exp(-bD_{iso}) + (1 - f) \exp(-bg_i Dg_i)] \quad (1)$$

where s_0 is the signal when no diffusion sensitization gradient is applied, f is the volume fraction of free water contamination, D is the diffusion tensor of the tissue, b is a parameter that depends on the diffusion gradient shape, g_i is the diffusion gradient direction and D_{iso} is the free water isotropic diffusion coefficient which is set to $3.0 \times 10^{-3} mm^2/s$ [11].

Implementation of fitting algorithms

Since no source implementation was previously provided by Hoy and colleagues, our implementation relies on the equations provided in the original article.

Weighted-Linear Least Square (WLS). Two errors were found in the equations describing the first proposed algorithm. Firstly, the free-water adjusted diffusion-weighted signal formula (original article’s Methods subsection “FWE-DTI”) should be written as:

$$y_{ik} = \ln \left\{ \frac{s_i - s_0 f_k \exp(-bD_{iso})}{(1 - f_k)} \right\} \quad (2)$$

instead of:

$$y_{ik} = \ln \left\{ \frac{s_i - s_0 \exp(-bD_{iso})}{(1 - f_k)} \right\} \quad (3)$$

where f_k is a grid search free water volume fraction sample.

Secondly, according to the general linear least squares solution [6], the parameters matrix is estimated using the weighted linear least squares solution of the free-water elimination model:

$$\gamma = (W^T S^2 W)^{-1} W^T S^2 y \quad (4)$$

instead of:

$$\gamma = (W^T S^2 W)(SW)^T S y \quad (5)$$

where γ contains the fwDTI model parameters $\gamma = [D_{xx}, D_{xy}, D_{yy}, D_{xz}, D_{yz}, D_{zz}, \ln(s_0)]$, y is a matrix containing the elements of y_{ik} computed from equation 2, S is a diagonal matrix with diagonal set to the s_i samples, and W is a matrix computed from the m diffusion-weighted directions g_i and b-values:

$$W = \begin{bmatrix} -b_1 g_{1x}^2 & -2b_1 g_{1x} g_{1y} & -b_1 g_{1y}^2 & -2b_1 g_{1x} g_{1z} & -2b_1 g_{1y} g_{1z} & -b_1 g_{1z}^2 & 1 \\ \vdots & \vdots & \vdots & \vdots & \vdots & \vdots & \vdots \\ b_m g_{mx}^2 & -2b_m g_{mx} g_{my} & -b_m g_{my}^2 & -2b_m g_{mx} g_{mz} & -2b_m g_{my} g_{mz} & -b_m g_{mz}^2 & 1 \end{bmatrix} \quad (6)$$

Relative to the original article, the elements of W have been re-ordered according to order of the diffusion tensor elements used in Dipy.

To ensure that the WLS method converges to the local minimum, f grid search sampling is performed over larger interval ranges relative to original article. Particularly, for the second and third iterations used to refine the parameters precision, f is resampled over intervals of 0.2 and 0.02 instead of interval sizes of 0.1 and 0.01 proposed by Hoy and colleagues. On the other hand, the sample step size was maintained to 0.01 and 0.001 respectively.

Moreover, since the WLS objective function is sensitive to the squared error of the model weights ($\omega_i = s_i$):

$$F_{WLS} = \frac{1}{2} \sum_{i=1}^m \left[\omega_i \left(y_i - \sum_{j=1}^7 W_{ij} \gamma_j \right) \right]^2 \quad (7)$$

when evaluating which (f, D_{tissue}) pair is associated with smaller residuals the NLS objective function is used instead:

$$F_{NLS} = \frac{1}{2} \sum_{i=1}^m \left[s_i - S_0 f \exp(-b_i D_{iso}) - (1 - f) \exp\left(-\sum_{j=1}^7 W_{ij} \gamma_j\right) \right]^2 \quad (8)$$

Similarly to the original article [5], this procedure is only used to obtain the initial guess for the free water elimination parameters, which were then used to initialize a fwDTI model non-linear convergence solver (see below).

Removing problematic first guess estimates. For cases where the ground truth free water volume fraction is near to one (i.e. voxels containing only free water), the tissue's diffusion tensor component can erroneously fit the free water diffusion signal and therefore the free water DTI model fails to identifying the signal as pure free water. In these cases, since both tissue and free water compartment can represent well the signal, the free water volume fraction can be arbitrarily estimated to any value of the range between 0 and 1 rather than being close to 1. To overcome this issue, before the use of the non-linear fitting procedure, Hoy et al. (2014) proposed to re-initialize the parameters initial guess when the tissue's mean diffusivity approaches the value of free water diffusion (tissue's MD $> 1.5 \times 10^{-3} mm^2/s$) [5]. In this study, these re-initialization settings are reviewed by accessing the fwDTI estimates for synthetic voxels than mostly contain free water diffusion and analysis the frequency that this problem arises as a function of ground truth f values (supplementary_notebook_1.ipynb). Based on this, the following parameters adjustments were done in our implementations when the initial tissue's mean diffusivity is higher than $1.5 \times 10^{-3} mm^2/s$: 1) free water volume fraction estimates are set to 1 indicating that the voxel is likely to be only related to free water diffusion; 2) the elements of the tissues diffusion tensor is set zero to avoid high tissue's mean diffusivity for high volume fraction estimates and to better indicate that tissue diffusion is practically absent.

Non-Linear Least Square Solution (NLS). To improve computation speed, instead of using the modified Newton's algorithm proposed in the original article, the

non-linear convergence was done using Scipy's wrapped modified Levenberg-Marquardt algorithm (function `scipy.optimize.leastsq` of [Scipy](#)).

To constrain the model parameters to plausible ranges, some variable transformations can be applied to the non-linear objective function. These were implemented as optional features that can be controlled through user-provided arguments. To restrict the range of the volume fraction to values between 0 and 1, the variable f in equation 8 can be replaced by $\sin(f_t - \pi/2)/2 + 1/2$ and non-linear convergence is performed as a function of f_t . To ensure that the diffusion tensor is positive definite, diffusion parameters can be converted to the Cholesky decomposition elements as described in [7].

In addition to the `scipy.optimize.leastsq` function, a more recently implemented version of Scipy's optimization function `scipy.optimize.least_square` (available as of Scipy's version 0.17) was also tested. The latter directly solves the non-linear problem with predefined constraints in a similar fashion to what is done in the original article, however our experiments showed that this procedure does not overcome the performance of `scipy.optimize.leastsq` in terms of accuracy, and requires more computing time (see `supplementary_notebook_2.ipynb` for more details).

To speed up the performance of the non-linear optimization procedure, the Jacobian of the free water elimination DTI model was analytically derived and incorporated in the non-linear procedure (for details of the Jacobian derivation see `supplementary_notebook_3.ipynb`). Due to increased mathematical complexity, our analytical Jacobian derivation is not compatible with the Cholesky decomposition. This variable transformation is therefore not used by default.

Implementation dependencies. In addition to the dependency on Scipy, both free water elimination fitting procedures require modules from Dipy [4], since these contain all necessary standard diffusion tensor fitting functions. Before the using the fwDTI fitting procedures proposed here, a Dipy's installation is therefore required (to install Dipy please follow the steps described in [dipy's website](#) or read the information the the README.md file of the repository subfolder code). In addition to Dipy's modules, the implemented procedures also requires the python package [NumPy](#), which is also a dependency of both Scipy and Dipy.

Simulation 1

In this study, the performance of the fwDTI fitting techniques is first assessed for five different tissue's diffusion tensor FA levels and for free water volume fraction contamination using the multi-tensor simulation module available in Dipy. This simulation corresponds to the results reported in Figure 5 of the original article [5].

The acquisition parameters for this first simulation are based on the previously optimized parameter set reported by Hoy et al. (2014) which consist in a total of 70 signal measured for diffusion b-values of 500 and 1500 s/mm^2 (each along 32 different diffusion directions) and for six b-value=0 s/mm^2 . As in the original article, the ground truth of tissue's diffusion tensor had a constant diffusion trace of $2.4 \times 10^{-3} mm^2/s$. The diffusion tensor's eigenvalues used for the five FA levels are reported in Table 1.

Table 1: Eigenvalues values used for the simulations

FA	0	0.11	0.22	0.3	0.71
λ_1	8.00×10^{-4}	9.00×10^{-4}	1.00×10^{-3}	1.08×10^{-3}	1.60×10^{-3}
λ_2	8.00×10^{-4}	7.63×10^{-4}	7.25×10^{-4}	6.95×10^{-4}	5.00×10^{-4}
λ_3	8.00×10^{-4}	7.38×10^{-4}	6.75×10^{-4}	6.25×10^{-4}	3.00×10^{-4}

For each FA value, eleven different degrees of free water contamination were evaluated (f values equally spaced from 0 to 1). To assess the procedure's robustness to

MRI noise, Rician noise with signal-to-noise ratio (SNR) of 40 relative to the b -value=0 s/mm^2 images was used, similarly to Hoy et al. (2014) [5]. For each FA and f -value pair, simulations were performed for 120 different diffusion tensor orientations which were repeated 100 times to make a total of 12000 simulated iterations for each FA and f -value pair [5].

Simulation 2

After evaluating the fitting procedures for the reported FA and f ground truth values, the optimal b -values for two-shell diffusion MRI acquisition are re-accessed. This second simulation corresponds to the original article's Figure 2 [5] in which b -value minimum is investigated from 200 to 800 s/mm^2 in increments of 100 s/mm^2 while b -value maximum is assessed from 300 to 1500 s/mm^2 in increments of 100 s/mm^2 . Similarly to Hoy et al. (2014), this simulation is done for a fixed f -value of 0.5 and FA of 0.71, corresponding to a typical MRI voxel in the boundary between CSF and white matter tissue. For each b -value pair, simulations are repeated 12000 times similarly to simulation 1 and fitting performances are quantified from the free water DTI's FA estimates, f estimates, and mean diffusivity estimates using the mean squared error ($MSE = \frac{1}{n} \sum_{i=1}^n (Y_i - \hat{Y})^2$, where $n=12000$, Y is the ground truth value of a diffusion measure, and Y_i is single measure estimate).

Simulation 3

To evaluate our implementations for different number of diffusion shells, different number of gradient directions, and different SNR levels, the lower panels of the original article's Figure 4 are replicated. For this last simulation, multi-compartmental simulations are performed for six different acquisition parameters sets that are summarized in Table 2.

Table 2: The six different acquisition parameter set tested

Number of shells	b -values (s/mm^2)	Directions per shell
2	500/1500	32 per shell
3	500/1000/1500	21/21/22
4	400/767/1133/1500	16 per shell
6	400/620/840/1060/1280/1500	10/10/10/10/10/14
8	300/471/643/814/986/1157/1329/1500	8 per shell
16	300/380/460/540/620/700/780/860/940/1020/1100/1180/1250/1340/1420/1500	4 per shell

Although Hoy et al. (2014) only reported the latter analysis for the higher FA level, here the lower FA values of 0 is also assessed. According to the original article, this optimization analysis is also done for the fixed f -value of 0.5. As the previous two simulations, tests are repeated 12000 times. Fitting performances are quantified using the mean squared error of the the free water DTI FA, f and MD estimates.

In vivo data

Similarly to the original article, the procedures are also tested using *in vivo* human brain data [12], that can be automatically downloaded by Dipy's functions (see `run_invivo_data.py` code script). The original dataset consisted of 74 volumes of images acquired for a b -value of 0 s/mm^2 and 578 volumes diffusion weighted images acquired along 16 diffusion gradient directions for b -values of 200 and 400 s/mm^2 and along 182 diffusion gradient directions for b -values of 1000, 2000 and 3000 s/mm^2 . In this study, only the data for b -values up to 2000 s/mm^2 are used to decrease the

impact of non-Gaussian diffusion effects which are not taken into account by the free water elimination model. We also processed the data with the standard DTI tensor model (as implemented in Dipy) in order to compare the results with the free water elimination model.

Results

The results from the first multi-compartmental simulations are shown in Figure 1. As reported in the original article, no FA bias are observed for large FA ground truth values and free water volume fractions f ranging around 0 to 0.7 (top panel of Figure 1). However, FA values seem to be overestimated for higher volume fractions. This bias is more prominent for lower FA values in which overestimations are visible from lower free water volume fractions. The lower panels of Figure 1 suggest that the free water elimination model produces accurate free water volume fraction for the full range of volume fraction ground truth values. All the features observed here are consistent with Figure 5 of the original article.

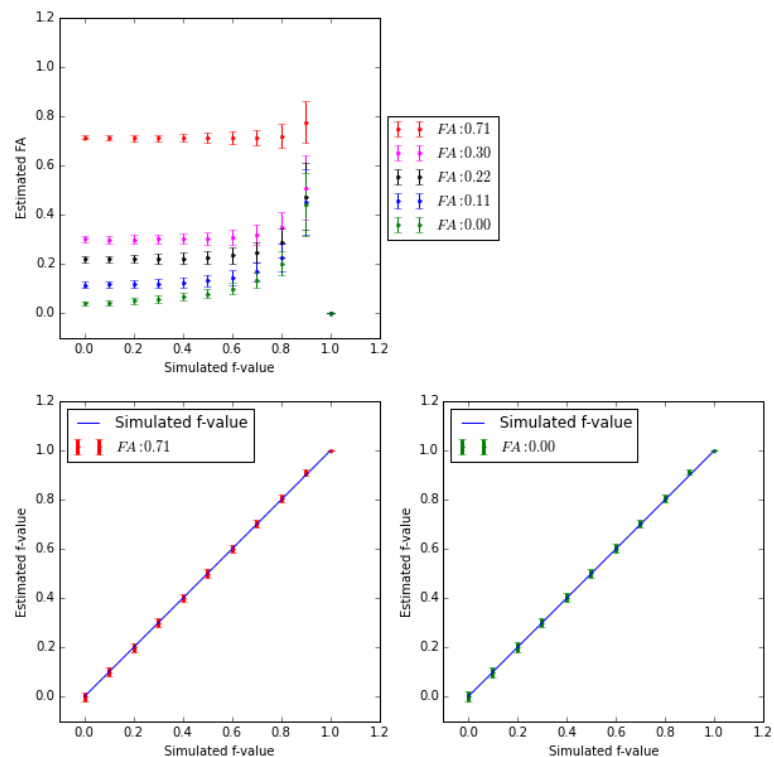


Figure 1: Fractional Anisotropy (FA) and free water volume fraction (f) estimates obtained with multi-compartmental simulations using the free water elimination fitting procedures. The top panel shows the FA median and interquartile range for the five different FA ground truth levels and plotted as a function of the ground truth water volume fraction. The bottom panels show the estimated volume fraction f median and interquartile range as a function of its ground truth values (right and left panels correspond to the higher and lower FA values, respectively). This figure reproduces Fig. 5 of the original article.

The re-evaluation of the optimal b-value for a two-shell acquisition scheme is shown

in Figure 2. For a better visualization of the optimal b-value pair, MSE is converted to its reciprocal inverse [5]. In this way, the optimal b-value pair corresponds to a inverse reciprocal mean squared error of 1 (IRMSE). Although our fwDTI fitting implementations seem to produce more stable IRMSE for all diffusion measures (note that colormaps were rescaled from 0.9 to 1), results of Figure 2 are consistent to the original article which suggests that the b-values pair 500-1500 s/mm^2 is the most adequate parameters for the fwDTI model fitting.




Figure 2: Inverse reciprocal mean squared errors (IRMSE) as a function of the minimum and maximum b-value for three different diffusion measures. For left to right panels, the IRMSE were computed from the tissue's fractional anisotropy, free water volume fraction estimates, and tissue's mean diffusivity. MD colormaps are in $\times 10^{-3} mm^2/s$. This figure reproduces Fig. 2 of the original article.

Figure 3 shows the mean squared errors as a function of the signal to noise ratio (SNR) for different set of acquisition parameters with different number of b-value shells and gradient directions. As reported in the original article [5], figure's upper panels show that the two-shell acquisition scheme provide better diffusion measure estimates when the ground truth FA is high. This suggests that for the fwDTI model fitting having larger number of diffusion gradient directions is more adequate than having a larger number of b-value with smaller number of diffusion gradient directions. With the exception of the MSE for FA estimates, results are consistent for the ground truth FA=0 (lower panels of Figure 3). The similar performances of fwDTI in estimating tissue's FA for the different parameter sets is expected. Since in this case tissue has isotropy diffusion, FA estimates should not depend on the number of sampled directions.

In vivo tensor statistics obtained from the free water elimination and standard DTI models are shown in Figure 4. Complete processing of all these measure took less than 1 hour on an average Desktop and Laptop PC (~2GHz processor speed), while the reported processing time by Hoy et al. was around 20 hours. The free water elimination model seems to produce higher values of FA in general and lower values of MD relative to the metrics obtained from the standard DTI model. These differences in FA and MD estimates are expected due to the suppression of the isotropic diffusion of free water. As similarly reported in the original article, high amplitudes of FA are observed in the periventricular gray matter which might be related to inflated values in voxels with high f values. These can be mitigated by excluding voxels with high free water volume fraction estimates (see supplementary_notebook_4.ipynb), similarly to what is suggested by Hoy and colleagues [5].

Conclusion

Despite the changes done to reduce the algorithm's execution time, the implemented procedures to solve the free water elimination DTI model have comparable performance in terms of accuracy to the original methods described by Hoy and colleagues [5]. Based on similar simulations used in the original article, our results confirmed that the free water elimination DTI model is able to remove confounding effects of fast




Figure 3: Mean squared errors (MSE) plotted as a function of the signal to noise ratio (SNR) for six different acquisition parameter sets. For left to right panels the MSE were computed from the tissue's fractional anisotropy estimates, free water volume fraction estimates and tissue's mean diffusivity. The upper panels of figure reproduces the lower panels of the original article Fig. 4 in which ground truth tissue's FA is set to 0.71. Lower panels show the analogous results for a ground truth tissue's FA of 0

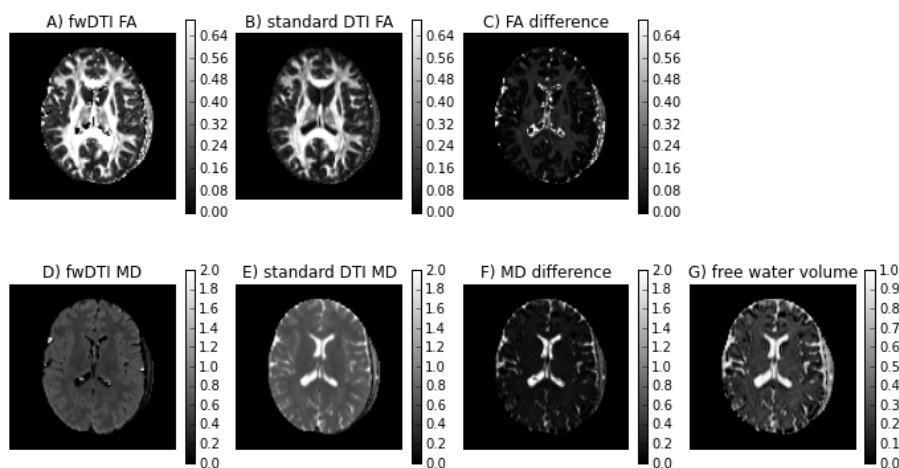


Figure 4: *In vivo* diffusion measures obtained from the free water DTI and standard DTI. The values of FA for the free water DTI model, the standard DTI model and their difference are shown in the top panels (A-C), while respective MD values are shown in the bottom panels (D-F). In addition the free water volume fraction estimated from the free water DTI model is shown in panel G. This figure reproduces Fig. 7 of the original article.

diffusion for typical FA values of brain white matter. Similarly to what was reported by Hoy and colleagues, the proposed procedures seem to generate biased values of FA for free water volume fractions near 1. Nevertheless, our results confirm that these problematic cases correspond to regions of the in vivo data that are not typically of interest in neuroimaging analysis (voxels associated with cerebral ventricles) and might be removed by excluding voxels with measured volume fractions above a reasonable threshold such as 0.7. This this study, it was also confirmed that for a fixed scanning time the fwDTI fitting procedures have better performance when data is acquired for diffusion gradient direction evenly distributed along two b-values of 500 and 1500 s/mm^2 .

Author Contributions

Conceptualization: RNH, AR, MMC. Data Curation: RNH, AR, EG, SSTJ. Formal Analysis: RNH. Funding Acquisition: RNH, AR. Investigation: RNH. Methodology: RNH, AR, EG. Project Administration: RNH, MMC, AR, EG. Resources: RNH, MMC, AR. Software: RNH, AR, ETP, EF, SSTJ. Supervision: MMC, AR. Validation: AR, SSTJ, EG. Visualization: RNH. Writing - Original Draft Preparation: RNH. Writing - Review & Editing: RNH, AR, MMC, ETP, SSTJ.

Acknowledgments

Rafael Neto Henriques was funded by Fundação para a Ciência e Tecnologia FCT/MCE (PIDDAC) under grant SFRH/BD/80114/2012.

Ariel Rokem was funded through a grant from the Gordon & Betty Moore Foundation and the Alfred P. Sloan Foundation to the University of Washington eScience Institute.

Thanks to Romain Valabregue, CENIR, Paris for providing the data used here.

References

- [1] P J Basser, J Mattiello, and D LeBihan. "Estimation of the effective self-diffusion tensor from the NMR spin echo". In: *J. Magn. Reson. B* 103.3 (Mar. 1994), pp. 247–254.
- [2] P J Basser, J Mattiello, and D LeBihan. "MR diffusion tensor spectroscopy and imaging". In: *Biophys. J.* 66.1 (Jan. 1994), pp. 259–267.
- [3] C Beaulieu. "The basis of anisotropic water diffusion in the nervous system – a technical review". In: *NMR Biomed.* 15.7-8 (Jan. 2002), pp. 435–455.
- [4] E Garyfallidis et al. "Dipy, a library for the analysis of diffusion MRI data". In: *Front. Neuroinform.* 8 (Feb. 2014), p. 8.
- [5] A R Hoy et al. "Optimization of a free water elimination two-compartment model for diffusion tensor imaging". In: *Neuroimage* 103 (Dec. 2014), pp. 323–333.
- [6] D K Jones and M Cercignani. "Twenty-five pitfalls in the analysis of diffusion MRI data". In: *NMR Biomed.* 23.7 (2010), pp. 803–820.
- [7] C G Koay et al. "Investigation of anomalous estimates of tensor-derived quantities in diffusion tensor imaging". In: *Magn. Reson. Med.* 55.4 (Apr. 2006), pp. 930–936.
- [8] C Metzler-Baddeley et al. "Frontotemporal connections in episodic memory and aging: A diffusion MRI tractography study". In: *J. Neurosci* 31.37 (Sept. 2011), pp. 13236–13245.
- [9] L J O'Donnell and O Pasternak. "Does diffusion MRI tell us anything about the white matter? An overview of methods and pitfalls." In: *Schizophr Res.* 161.1 (Jan. 2015), pp. 133–141.

- [10] N G Papadakis et al. "Study of the effect of CSF suppression on white matter diffusion anisotropy mapping of healthy human brain." In: *Magn. Reson. Med.* 48.2 (Aug. 2002), pp. 394–398.
- [11] O Pasternak et al. "Free water elimination and mapping from diffusion MRI." In: *Magn. Reson. Med.* 62.3 (Sept. 2009), pp. 717–730.
- [12] Valabregue Romain. *Diffusion MRI measured at multiple b-values*. <https://digital.lib.washington.edu/researchworks/handle/1773/33311>.